


# Mass Spectrum

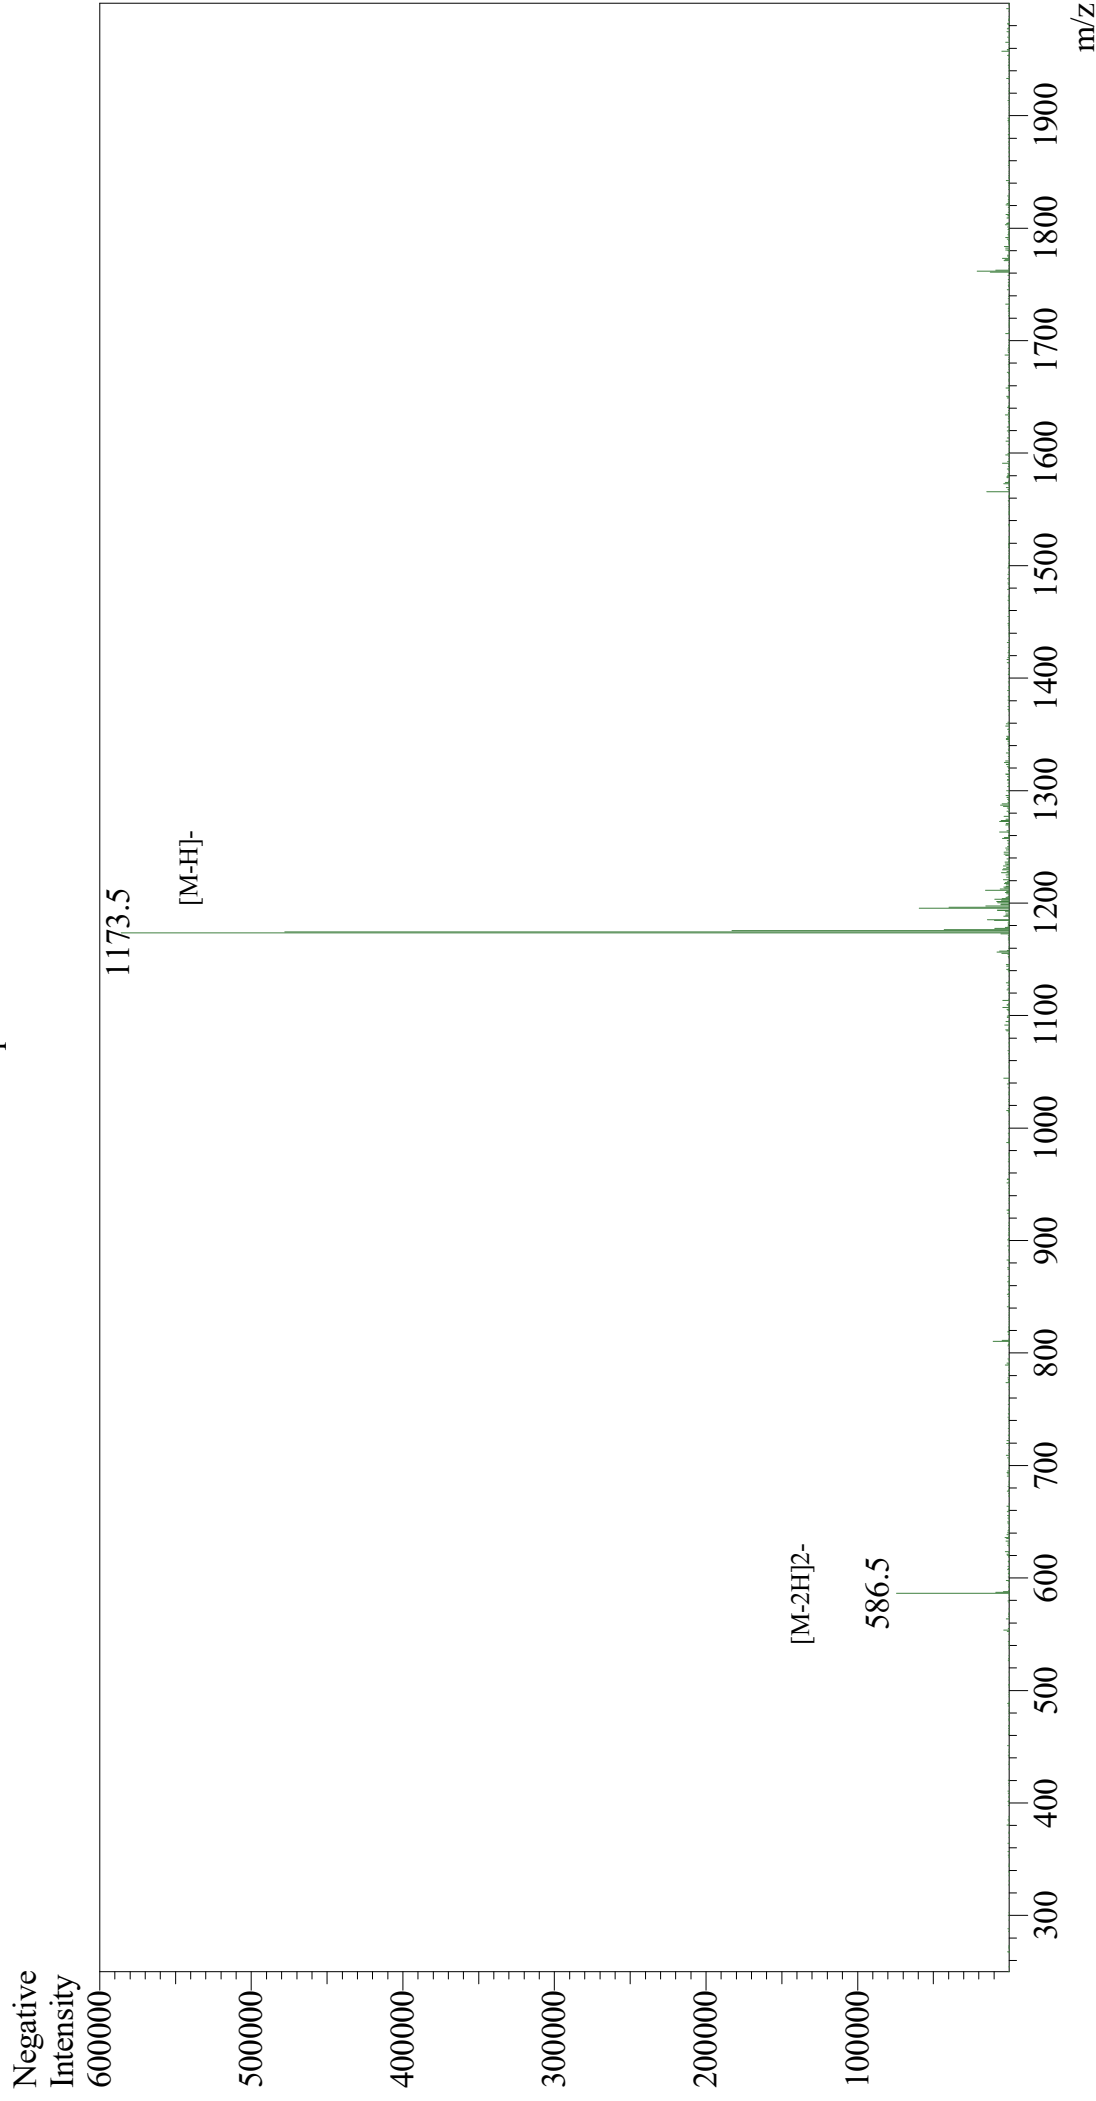

## Sample Information

User : Gary  
Month-Day Processed : 01/10/20  
Time Processed : 12:06:36 PM  
Injection Volume : 0.4  
Sample Name : mTRP-2(180-188)  
Cat No. : RP20250  
Lot No. : E5557220A  
Theoretical MW : 1175.34  
Observed MW : 1174.5

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : -3.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50%H2O/50%MeOH