

Sample Name: Hexa-His
 Cat No. : RP11737
 Lot No. : E3385419L
 Time Processed: 10:30:20 AM
 Month-Day-Year Processed :12/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	0
33.00	Pumps	Solvent B Conc.	0
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

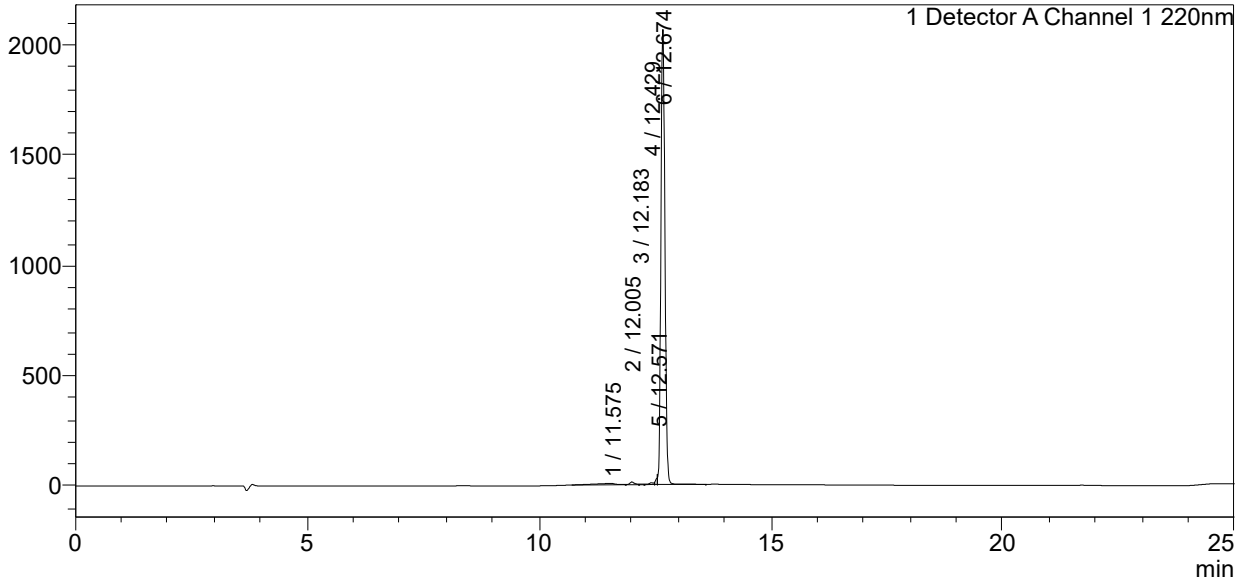

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.575	206919	6633	1.602
2	12.005	90495	12222	0.701
3	12.183	14094	2241	0.109
4	12.429	51932	8124	0.402
5	12.571	143453	35408	1.111
6	12.674	12409462	2065540	96.076
Total		12916356	2130167	100.000