

Sample Name :Gastric Inhibitory Peptide (GIP), human
 Cat. No. : RP10795
 Lot. No. : PE2911901
 Time Processed : 13:06:58
 Month-Day-Year Processed : 02/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

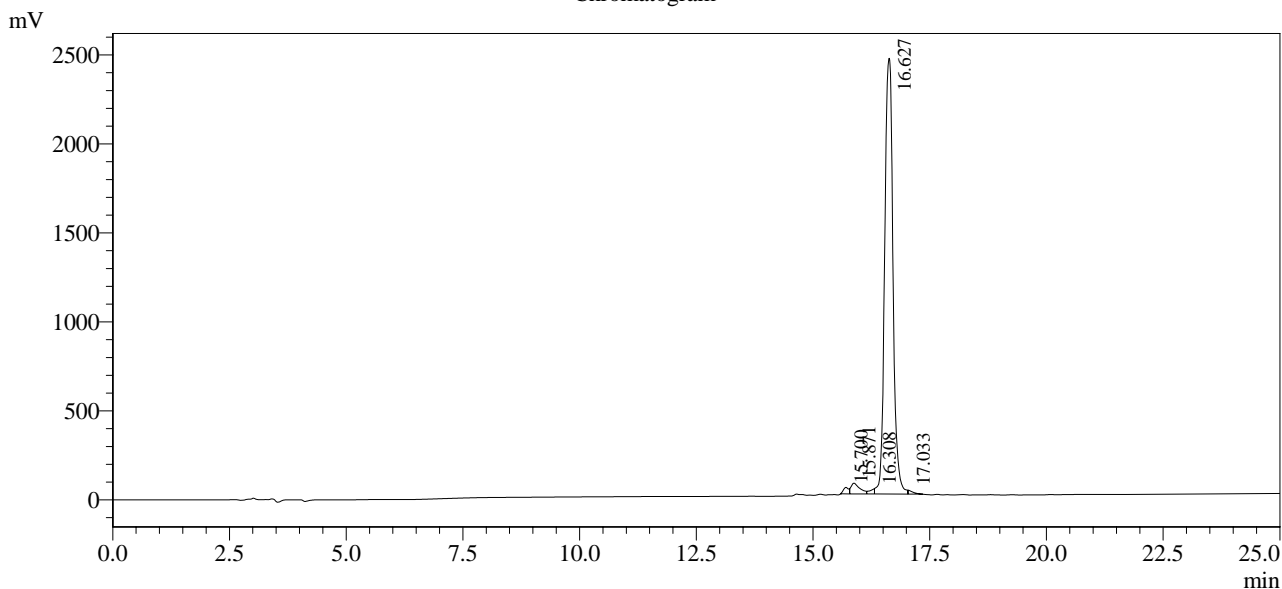

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.700	288377	36264	0.910
2	15.871	788445	60216	2.487
3	16.308	208157	29488	0.657
4	16.627	30270078	2448664	95.470
5	17.033	151225	22578	0.477
Total		31706281	2597210	100.000