

Sample Name : DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : PE7191701

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	1	
25.00	Pumps	Pump B Conc.	50	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	1	
37.00	Pumps	Pump B Conc.	1	
37.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

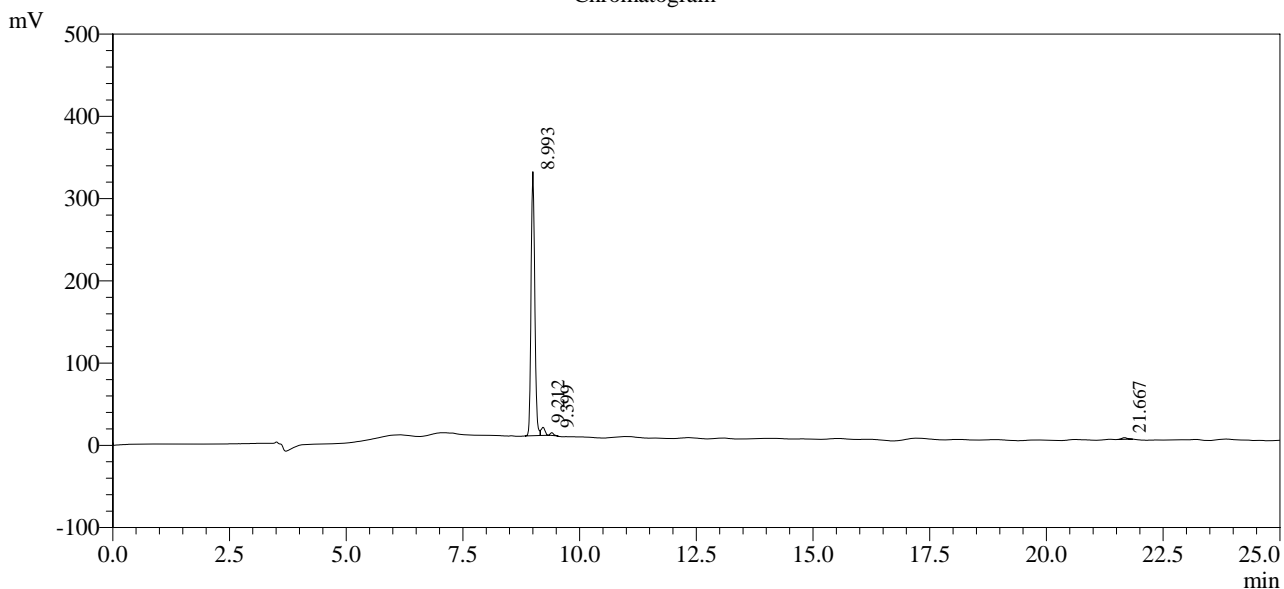

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.993	1792111	321080	95.302
2	9.212	55895	9904	2.972
3	9.399	16735	3420	0.890
4	21.667	15711	1947	0.836
Total		1880452	336351	100.000