

Sample Name :Gastric Inhibitory Peptide (GIP), human
 Cat No. : RP10795 Lot No. : PE2441810
 Time Processed : 19:55:34
 Month-Day-Year Processed : 10/15/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

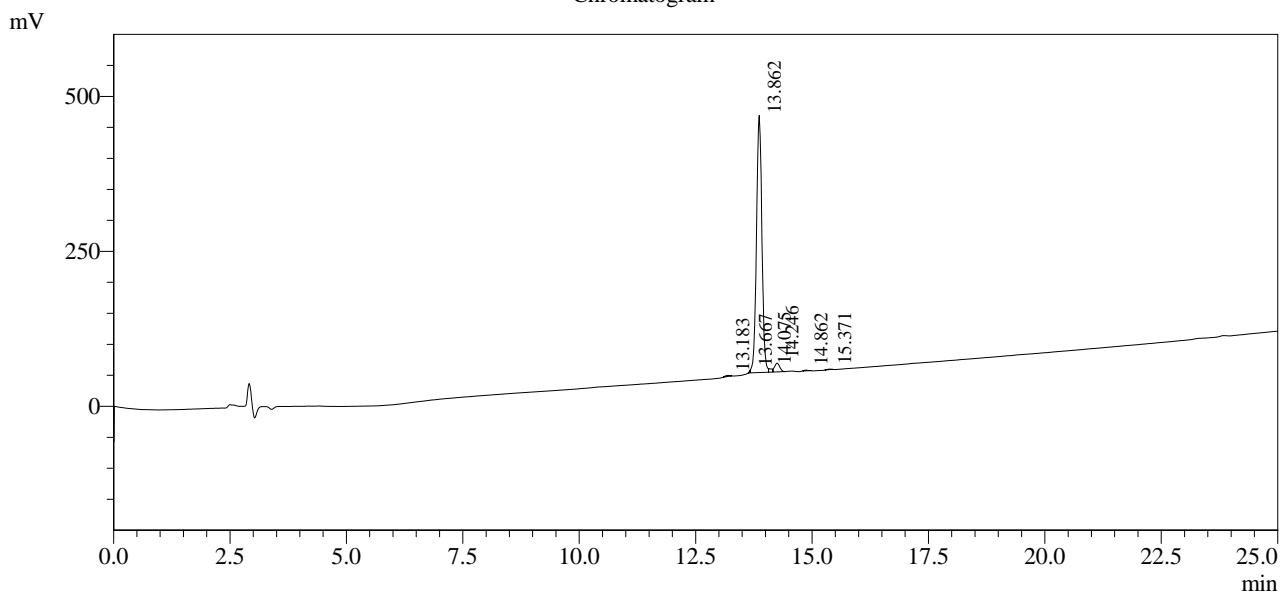

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.183	10663	1676	0.304
2	13.667	7693	3791	0.219
3	13.862	3344192	414791	95.350
4	14.075	27533	5320	0.785
5	14.246	105529	13962	3.009
6	14.862	6348	1108	0.181
7	15.371	5318	899	0.152
Total		3507276	441547	100.000