

Sample Name :LAH4
 Cat No. :RP20096
 Lot No. :E7329121A
 Time Processed :6:32:31
 Month-Day-Year Processed :01/16/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

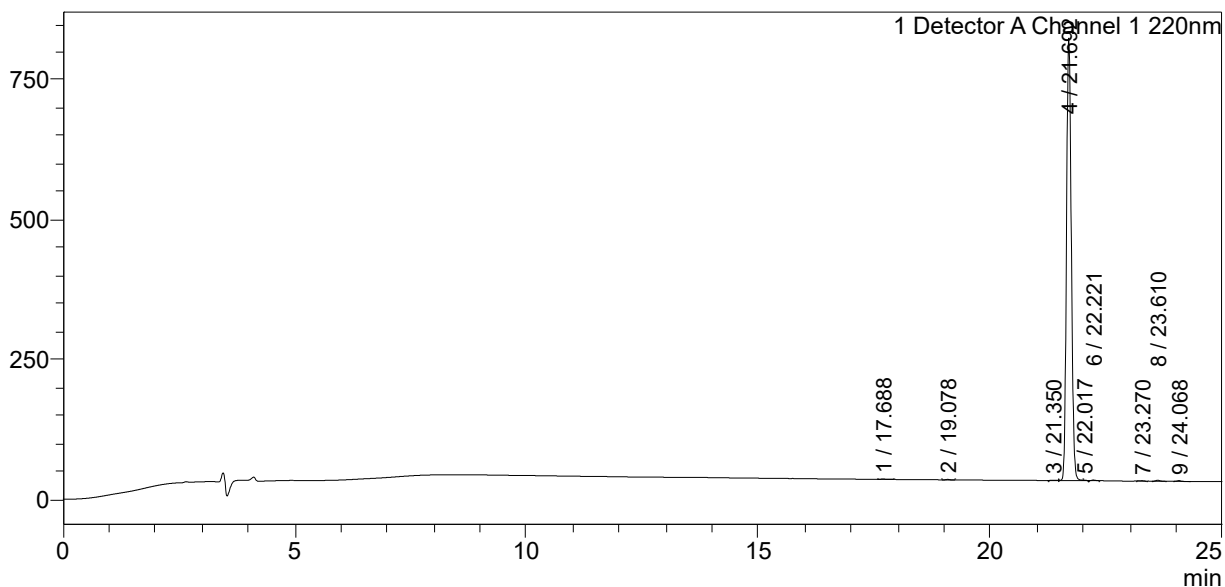

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.688	3763	663	0.065
2	19.078	4334	881	0.075
3	21.350	3479	330	0.060
4	21.692	5719382	791982	99.325
5	22.017	1097	269	0.019
6	22.221	6034	1151	0.105
7	23.270	2549	538	0.044
8	23.610	9786	1780	0.170
9	24.068	7834	1445	0.136
Total		5758257	799039	100.000