

Sample Name : Glucagon-Like Peptide (GLP) II, human
 Cat No. : RP10769
 Lot No. : E6860420H
 Time Processed : 10:46:38
 Month-Day-Year Processed : 08/06/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

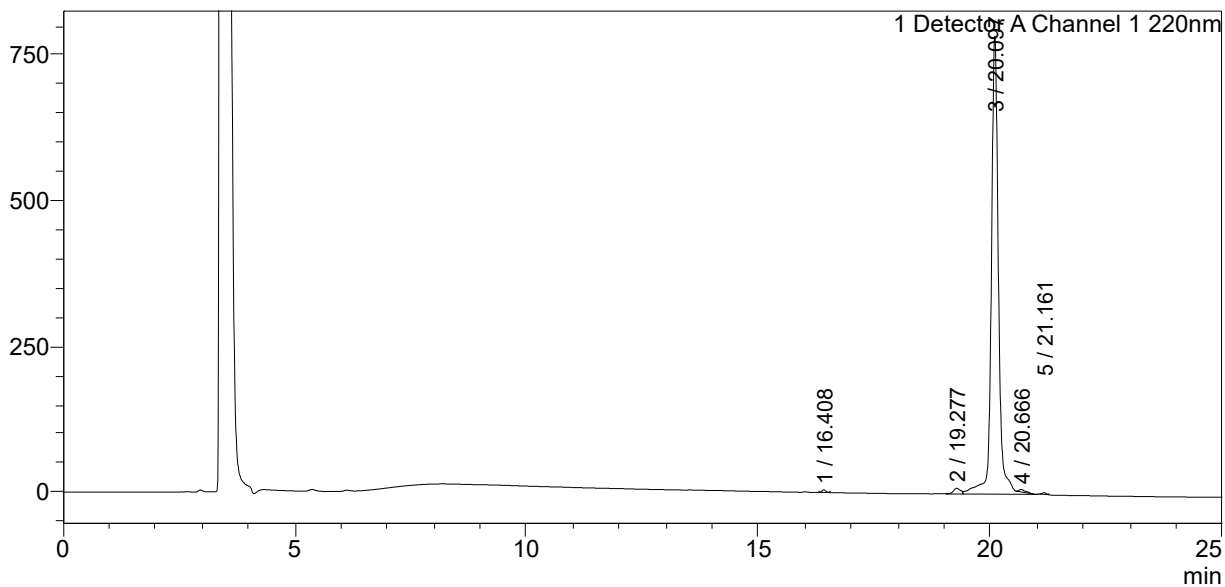

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.408	25041	4350	0.289
2	19.277	108318	9655	1.252
3	20.097	8456627	786165	97.767
4	20.666	41967	4213	0.485
5	21.161	17840	3011	0.206
Total		8649793	807394	100.000