

Sample Name : Melittin,honey bee
 Cat.No : RP20415
 Lot.No : E3427621B
 Time Processed: 1:39:41
 Year-Month-Day: 2021/2/24

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010015

<Chromatogram>

mV

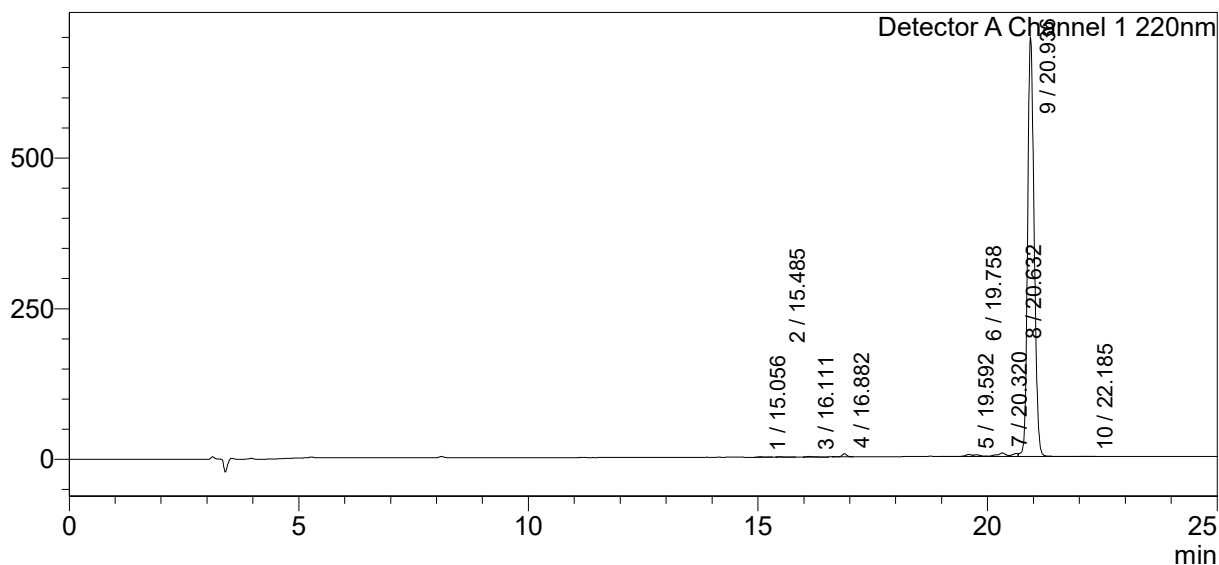

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.056	5858	828	0.082
2	15.485	3783	559	0.053
3	16.111	6950	1008	0.098
4	16.882	31160	4954	0.438
5	19.592	32060	3093	0.451
6	19.758	27358	2762	0.384
7	20.320	77876	5747	1.094
8	20.632	42500	4915	0.597
9	20.936	6886545	696329	96.779
10	22.185	1682	206	0.024
Total		7115772	720402	100.000