

Sample Name :DYKDDDDK Peptide
 Cat No.: RP10586
 Lot No.: E4412421A
 Time Processed :15:51:26
 Month-Day-Year Processed :01/30/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	0
5.00	Pumps	Solvent B Conc.	0
20.00	Pumps	Solvent B Conc.	30
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	0
40.00	Pumps	Solvent B Conc.	0
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

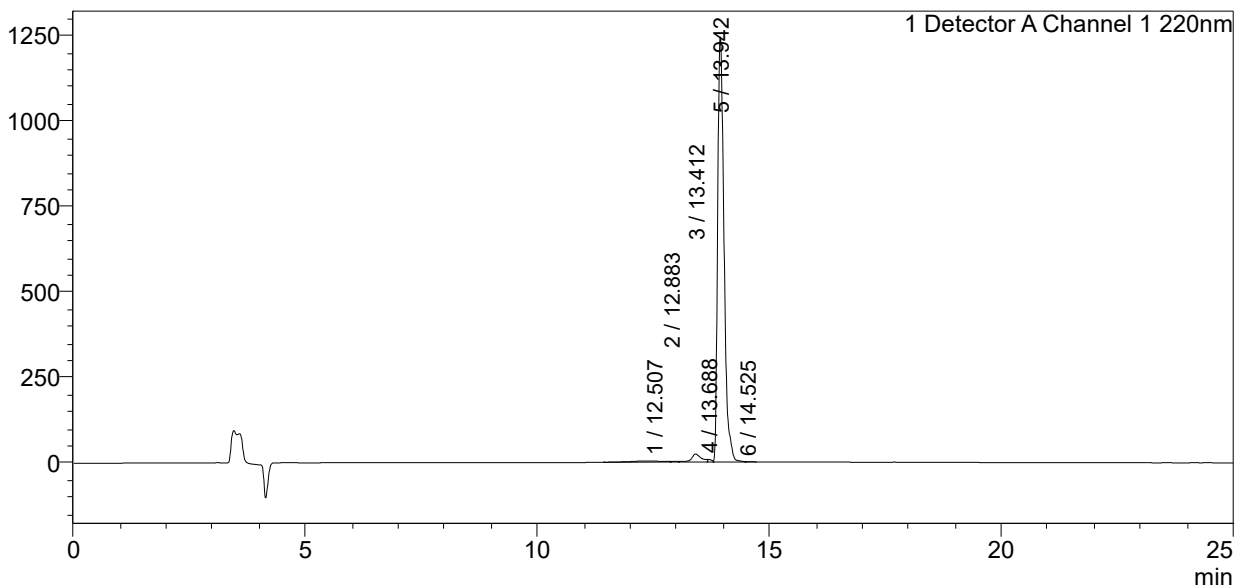

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.507	170484	3598	1.368
2	12.883	23454	2128	0.188
3	13.412	340857	23402	2.734
4	13.688	56148	7569	0.450
5	13.942	11867840	1243479	95.201
6	14.525	7365	872	0.059
Total		12466149	1281049	100.000