

Sample Name :mTRP-2(180-188)  
 Cat No. : RP20250  
 Lot No. : E4260719K  
 Time Processed : 17:11:16  
 Month-Day-Year Processed : 11/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

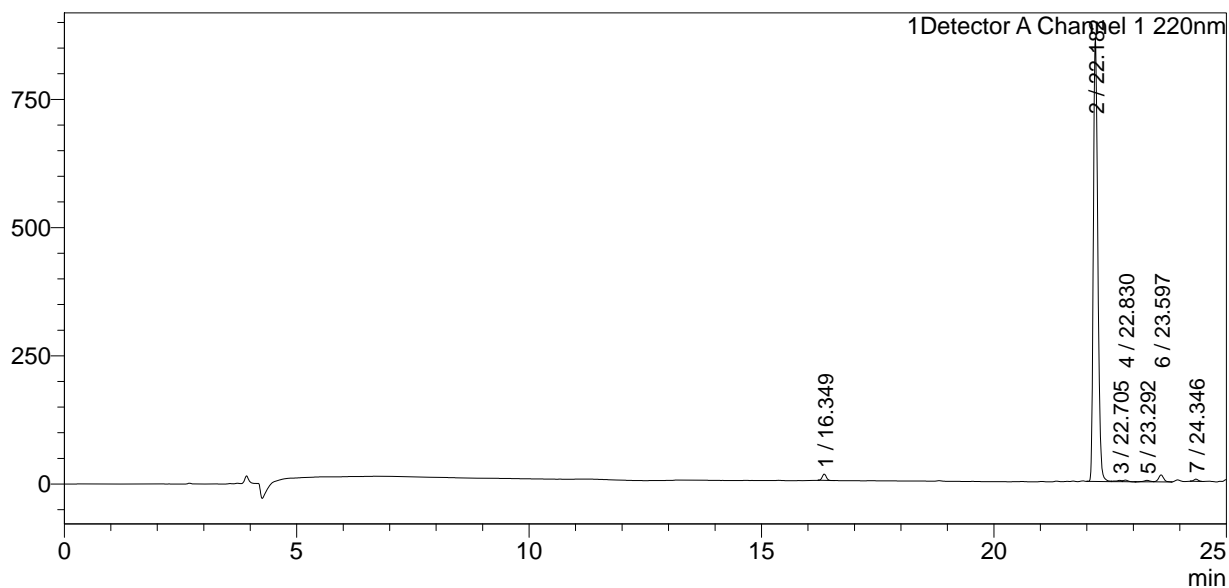

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.349	74262	12298	1.233
2	22.182	5740520	863698	95.315
3	22.705	23186	2641	0.385
4	22.830	22739	3198	0.378
5	23.292	29281	3020	0.486
6	23.597	104631	13705	1.737
7	24.346	28052	4346	0.466
Total		6022671	902905	100.000