

Sample Name : CEF20
 Cat. No. : RP11781
 Lot. No. : E12474201
 Time Processed : 4:45:15

Month-Day-Year Processed : 09/19/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010141

<Chromatogram>

mV

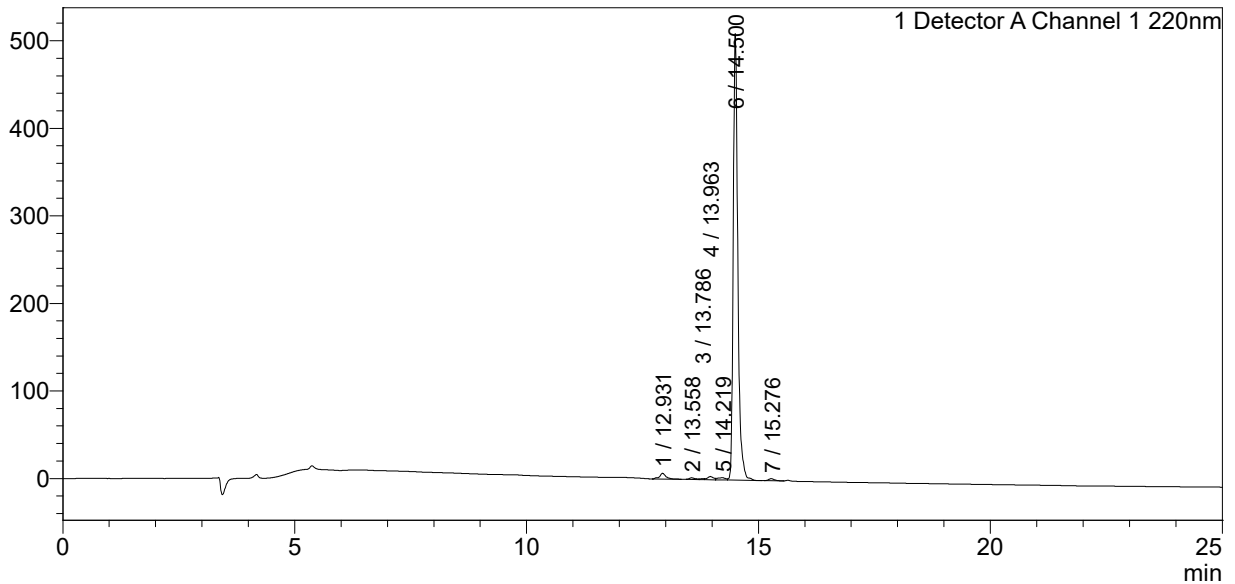

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.931	63781	6613	1.738
2	13.558	16132	1818	0.440
3	13.786	6127	940	0.167
4	13.963	33510	3665	0.913
5	14.219	31064	2524	0.846
6	14.500	3497225	510201	95.293
7	15.276	22143	2412	0.603
Total		3669982	528173	100.000