


Mass Spectrum

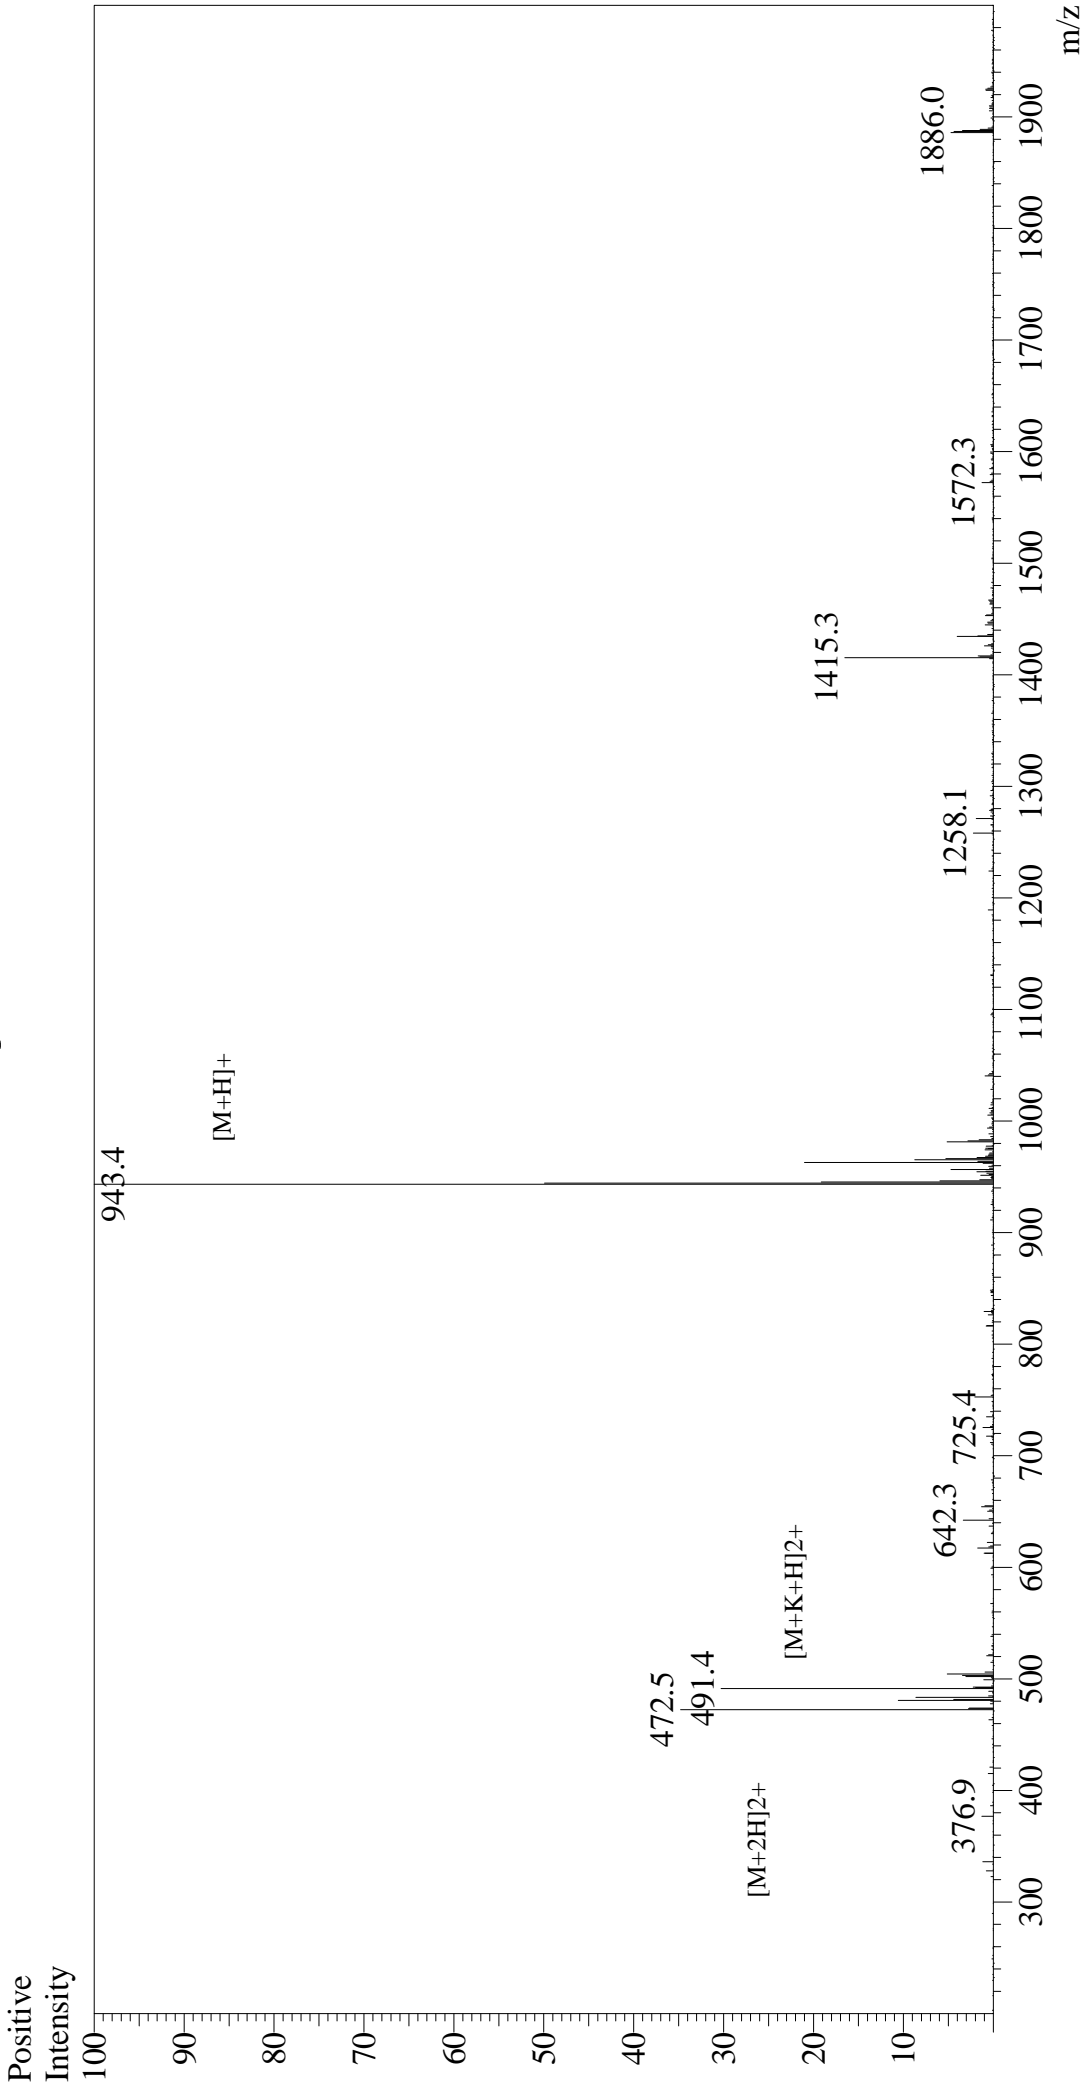

Sample Information
Month-Day Processed : 09/19/20
Time Processed : 0:13:02
Injection Volume : 0.3
Sample Name : CEF20
Cat. No. : RP11781
Lot. No. : E1247420I
Theoretical MW : 943.18
Observed MW : 942.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200
Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H2O/50% MeOH