

Sample Name: Melittin, honey bee
 Cat No. : RP20415
 Lot No. : E1314621F
 Time Processed : 17:18:36
 Month-Day-Year Processed : 06/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

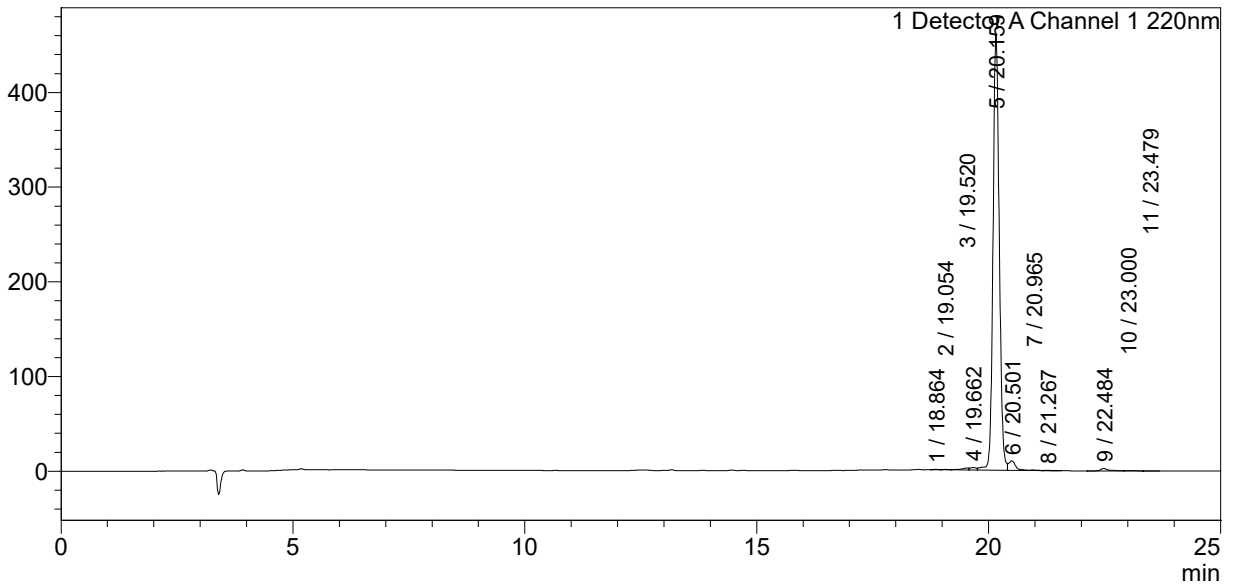

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	18.864	1955	339	0.043
2	19.054	2804	293	0.062
3	19.520	23376	2051	0.517
4	19.662	25185	2591	0.557
5	20.159	4307318	461174	95.338
6	20.501	107691	9993	2.384
7	20.965	1210	170	0.027
8	21.267	1618	143	0.036
9	22.484	37781	2700	0.836
10	23.000	6563	413	0.145
11	23.479	2425	157	0.054
Total		4517927	480023	100.000