

Sample Name :Hexa-His
 Cat. No. : RP11737
 Lot. No. : E4315019L
 Time Processed :8:02:13
 Month-Day-Year Processed : 12/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

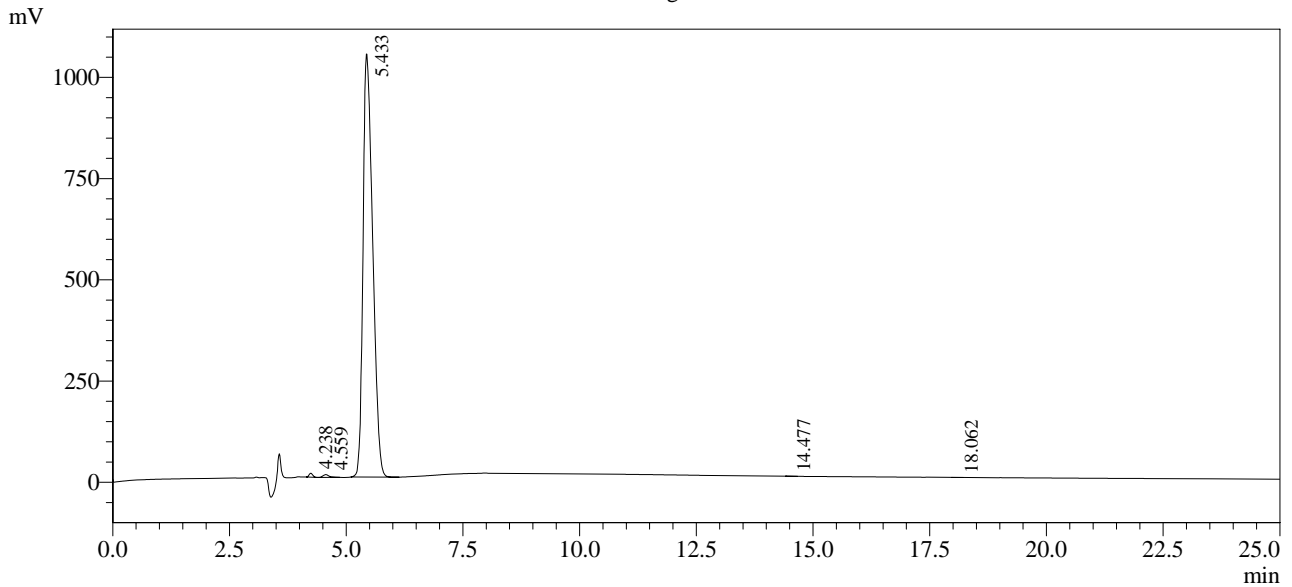

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.238	52332	9553	0.345
2	4.559	62910	6883	0.415
3	5.433	15037058	1045151	99.213
4	14.477	1161	171	0.008
5	18.062	2883	455	0.019
Total		15156343	1062212	100.000