

Sample Name : β -Amyloid (25-35)
 Cat No.: RP10008
 Lot No.: E6073820C
 Time Processed :8:50:25
 Month-Day-Year Processed :03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010014

<Chromatogram>

mV

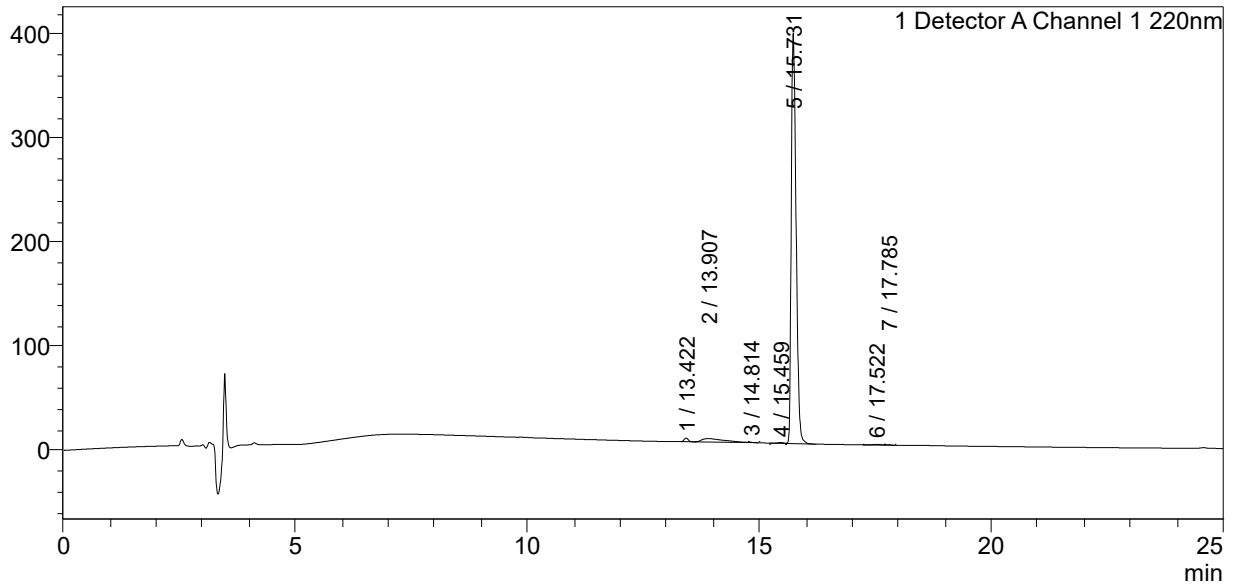

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.422	22165	3578	0.737
2	13.907	107657	3377	3.581
3	14.814	1221	181	0.041
4	15.459	8713	942	0.290
5	15.731	2857454	394978	95.054
6	17.522	6545	540	0.218
7	17.785	2387	441	0.079
Total		3006141	404037	100.000