

Sample Name : IRBP (1-20), human
 Cat. No. : RP20269
 Lot. No. : PE1901810
 Time Processed :13:59:17
 Month-Day-Year Processed :10/18/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
10.00	Pumps	Pump A B.Conc	35	
35.00	Pumps	Pump A B.Conc	95	
41.00	Pumps	Pump A B.Conc	95	
41.01	Pumps	Pump A B.Conc	5	
50.00	Pumps	Pump A B.Conc	5	
50.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

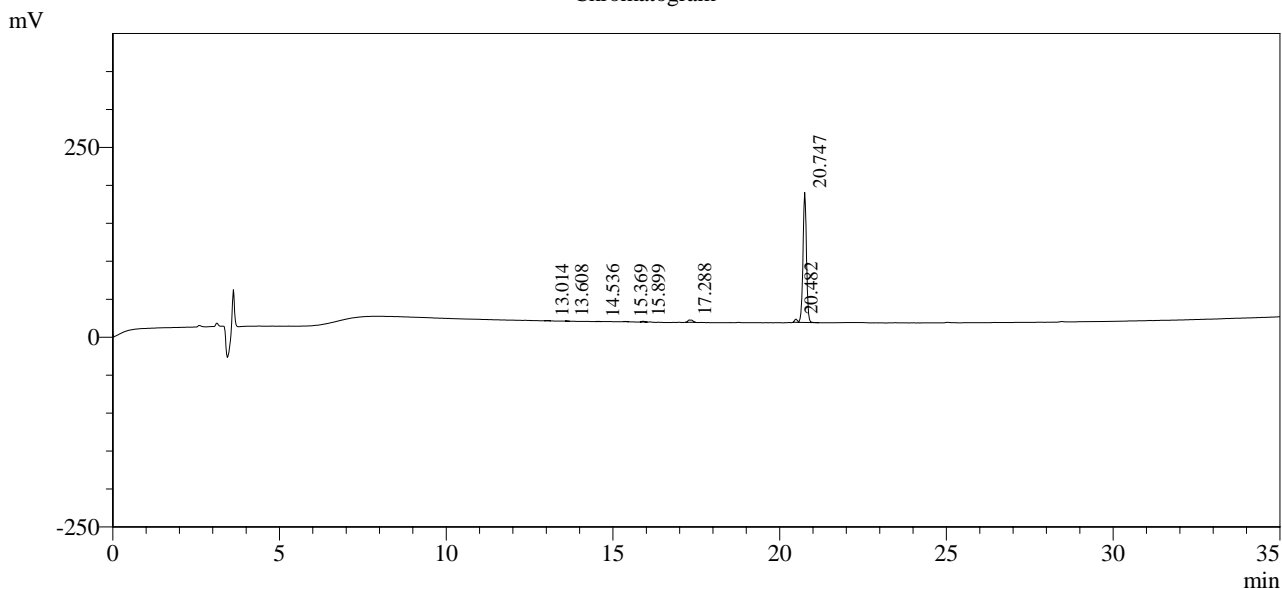

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.014	1224	188	0.093
2	13.608	434	135	0.033
3	14.536	985	189	0.075
4	15.369	1069	236	0.081
5	15.899	6101	1155	0.464
6	17.288	30553	3023	2.324
7	20.482	24144	4125	1.837
8	20.747	1249917	171402	95.092
Total		1314427	180453	100.000