

Sample Name : GLP-1 (7-36), amide, human  
 Cat. No. : RP10773  
 Lot. No. : PE0671805

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

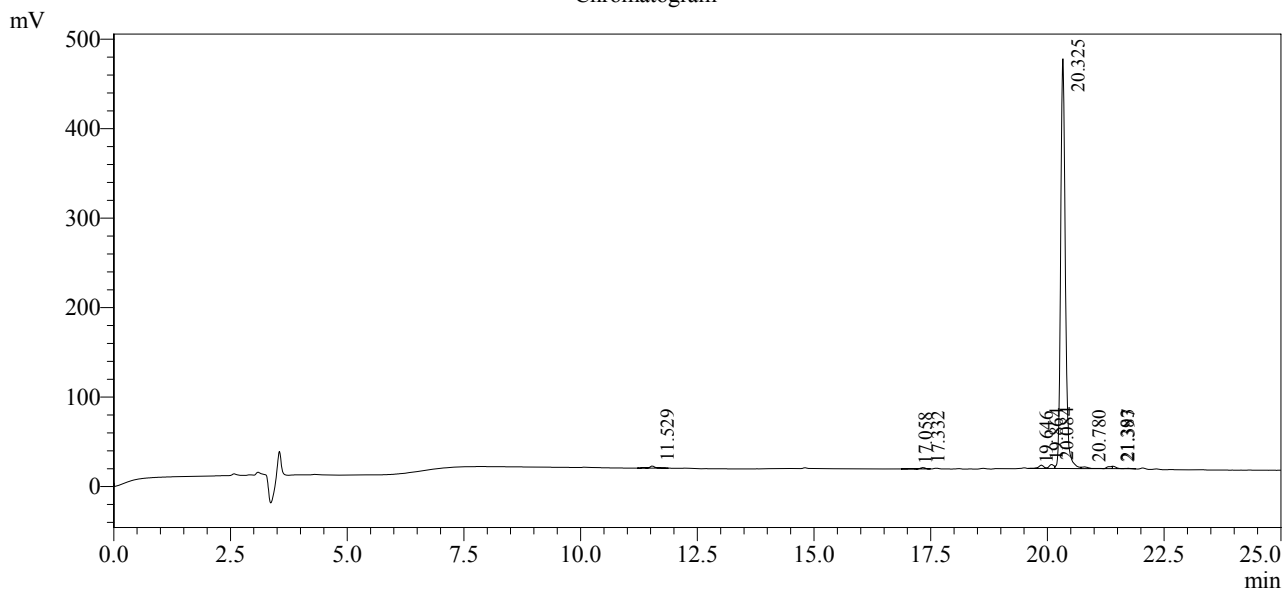

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.529	21940	2368	0.654
2	17.058	2286	237	0.068
3	17.332	11425	1520	0.340
4	19.646	694	173	0.021
5	19.864	28240	3796	0.842
6	20.084	31558	4503	0.940
7	20.325	3202860	457692	95.442
8	20.780	19463	1919	0.580
9	21.383	18857	2637	0.562
10	21.397	18504	2765	0.551
Total		3355826	477608	100.000