

Sample Name :GRGDSPC
 Cat No :RP20283
 Lot No :E3031921D
 Time Processed :4:31:40
 Month-Day-Year Processed :04/19/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

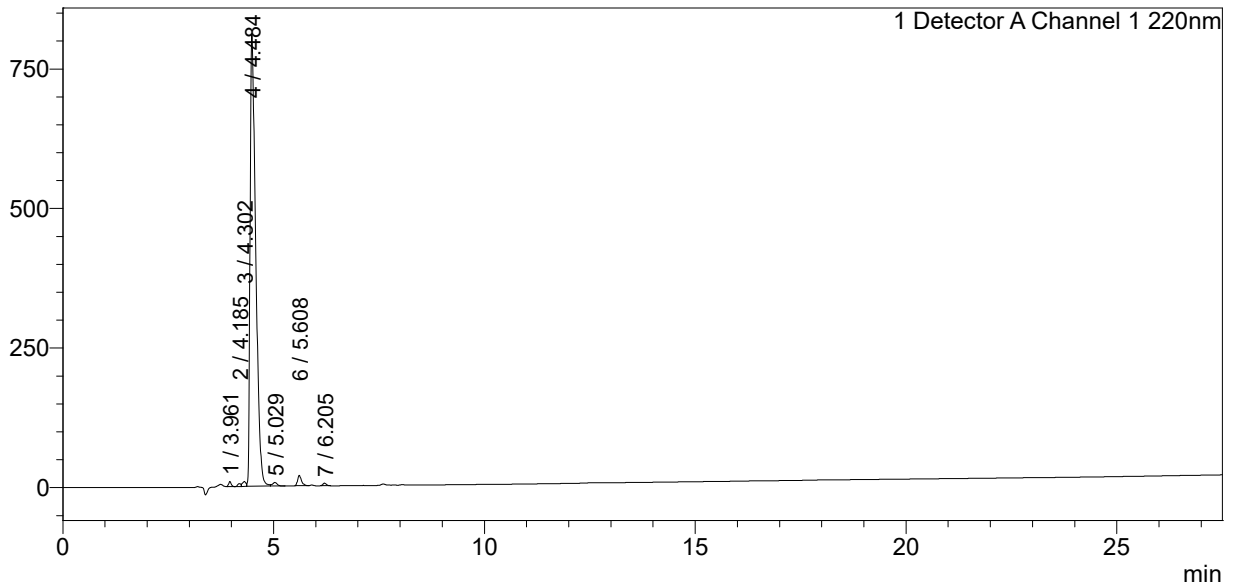

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	3.961	36972	9068	0.471
2	4.185	28086	5237	0.358
3	4.302	50346	8683	0.641
4	4.484	7545297	810697	96.105
5	5.029	47811	6166	0.609
6	5.608	118251	18726	1.506
7	6.205	24332	4381	0.310
Total		7851095	862959	100.000