

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide

Cat No. : RP21087

Lot No. : E9538621B

Time Processed :1:20:18 PM

Month-Day-Year Processed :03/09/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010140

<Chromatogram>

mV

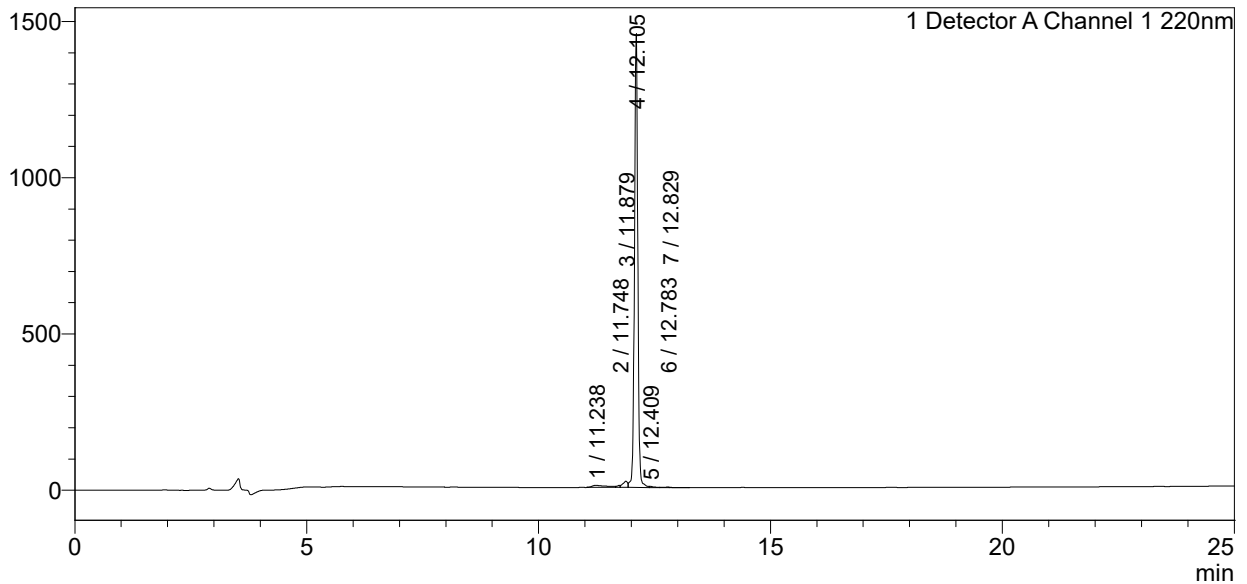

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.238	147617	6282	1.920
2	11.748	31315	6748	0.407
3	11.879	146788	20388	1.909
4	12.105	7320651	1452743	95.202
5	12.409	25300	3470	0.329
6	12.783	11738	1769	0.153
7	12.829	6195	971	0.081
Total		7689604	1492370	100.000