

Sample Name :OVA Peptide (323-339)  
 Cat. No. : RP10610  
 Lot. No. : E4404021E

Time Processed :8:13:23 PM  
 Month-Day-Year Processed :05/30/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm  
 Equipment: ZJ19010324

<Chromatogram>

mV

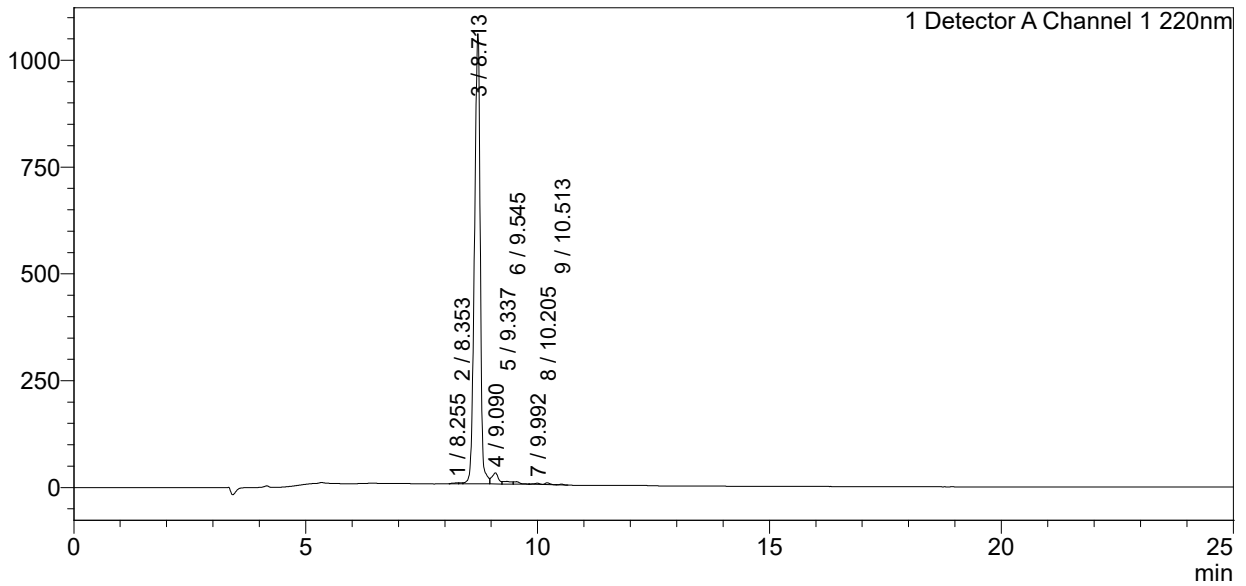

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.255	18945	2313	0.197
2	8.353	12925	2510	0.135
3	8.713	9119537	1054044	95.040
4	9.090	255796	26243	2.666
5	9.337	79032	6176	0.824
6	9.545	49957	5585	0.521
7	9.992	19390	2522	0.202
8	10.205	28255	4339	0.294
9	10.513	11590	1999	0.121
Total		9595427	1105731	100.000