

Sample Name :MDYKDHDGDYKDHDIDYKDDDDK peptide  
 Cat No.: RP21087  
 Lot No.: PE2941820E  
 Time Processed :9:52:27  
 Month-Day-Year Processed :05/15/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

### <Chromatogram>

mV

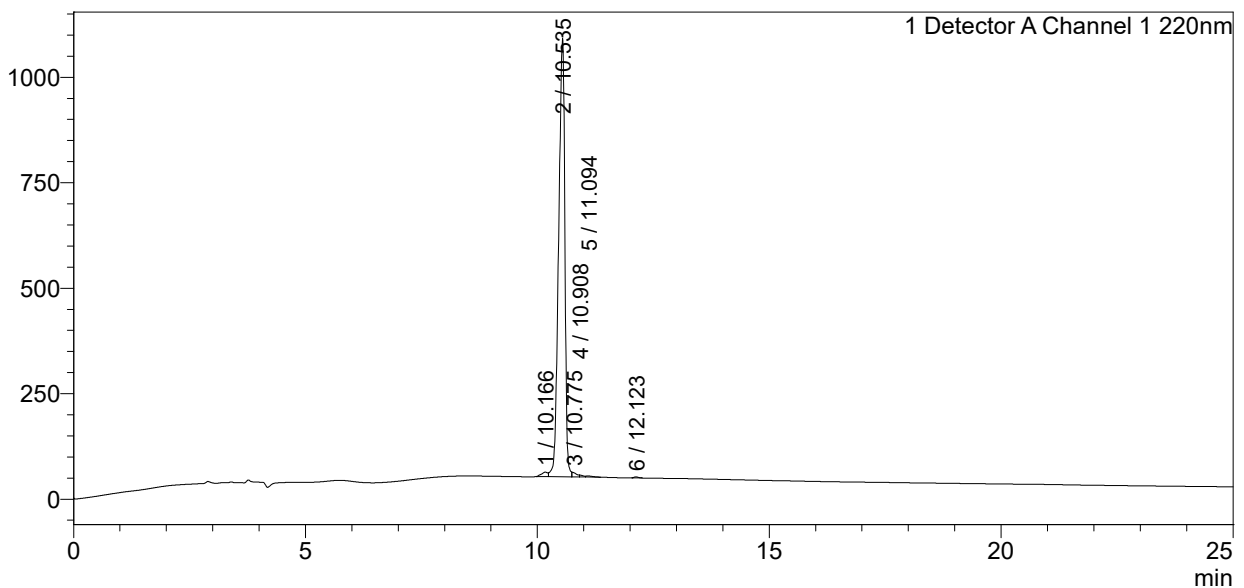

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.166	107632	10763	1.086
2	10.535	9668399	1004108	97.535
3	10.775	75125	10799	0.758
4	10.908	23811	4449	0.240
5	11.094	23444	2685	0.237
6	12.123	14350	2347	0.145
Total		9912760	1035152	100.000