

Sample Name : c-Myc Peptide
 Cat. No. : RP11731
 Lot. No. : E2873820B
 Time Processed : 8:46:02
 Month-Day-Year Processed : 03/15/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

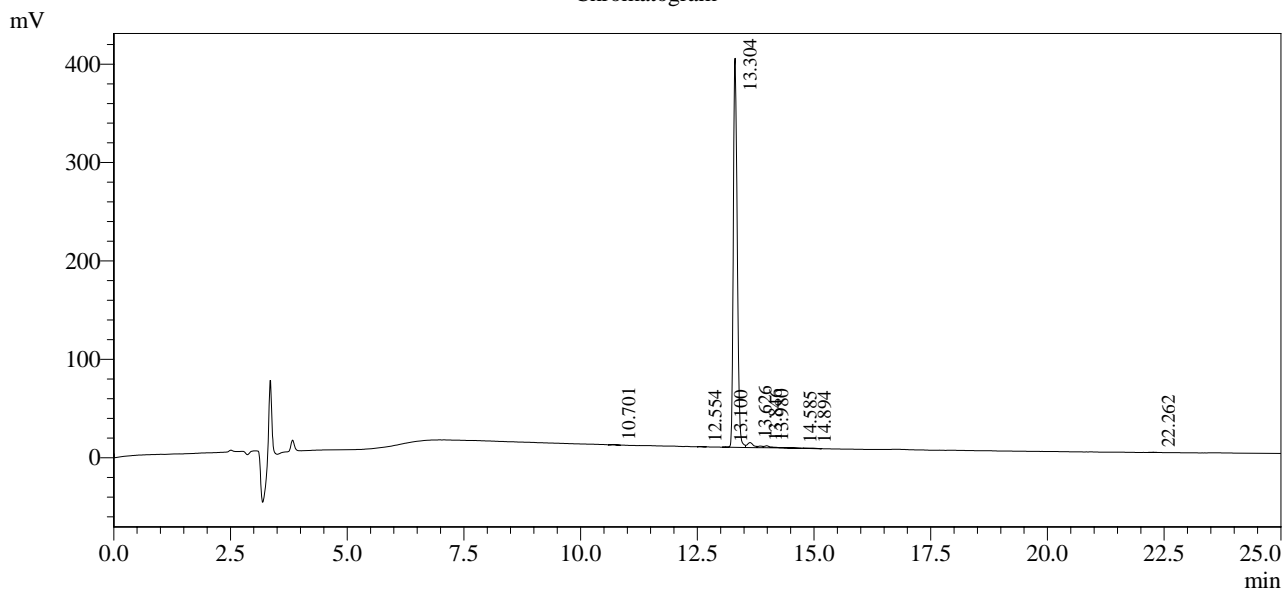

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.701	2786	494	0.116
2	12.554	1581	299	0.066
3	13.100	1052	252	0.044
4	13.304	2311150	395424	96.079
5	13.626	44503	4988	1.850
6	13.846	11517	1596	0.479
7	13.980	23009	2026	0.957
8	14.585	2596	388	0.108
9	14.894	5680	636	0.236
10	22.262	1597	208	0.066
Total		2405472	406312	100.000