

Sample Name :Hexa-His  
 Cat. No. : RP11737  
 Lot. No. :E5643319H  
 Time Processed : 7:24:38  
 Month-Day-Year Processed :08/02/2019  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:SS-CM-0286

Chromatogram

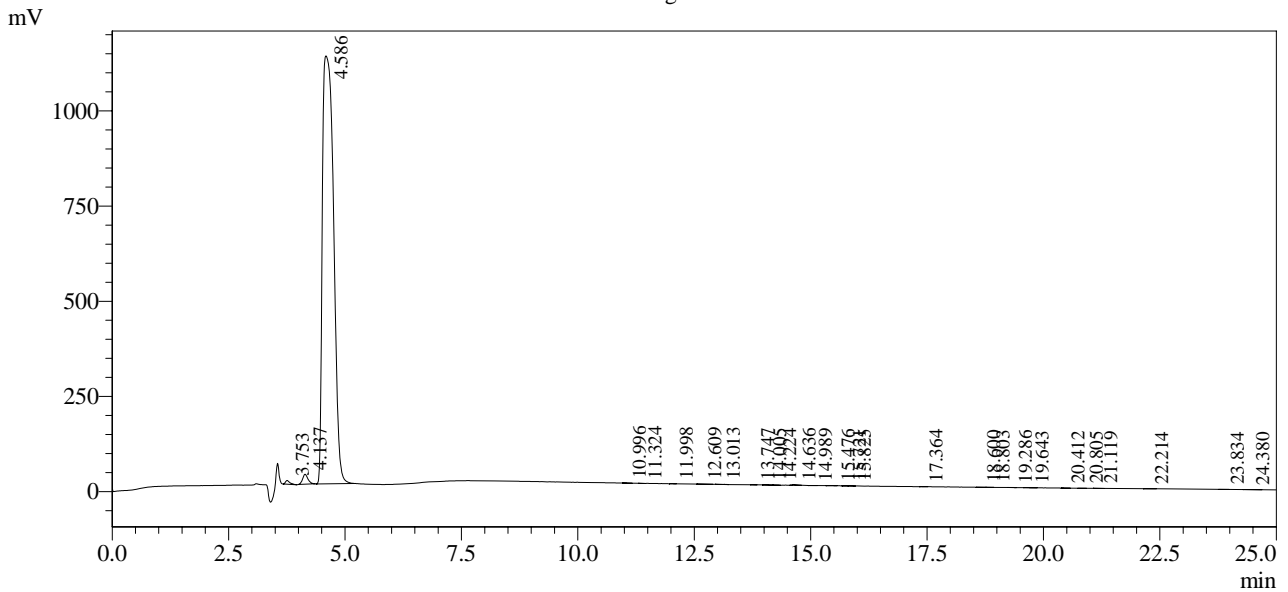

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	3.753	63358	9926	0.332
2	4.137	205206	26126	1.074
3	4.586	18786670	1123946	98.332
4	10.996	1129	160	0.006
5	11.324	1040	209	0.005
6	11.998	1541	347	0.008
7	12.609	3205	244	0.017
8	13.013	4277	480	0.022
9	13.747	1180	316	0.006
10	14.005	2029	226	0.011
11	14.224	1089	169	0.006
12	14.636	9463	1708	0.050
13	14.989	1349	209	0.007
14	15.476	2386	323	0.012
15	15.721	1241	225	0.006
16	15.825	1131	233	0.006
17	17.364	1473	260	0.008
18	18.600	1075	210	0.006
19	18.803	1009	215	0.005
20	19.286	1050	188	0.005
21	19.643	1984	195	0.010
22	20.412	1153	128	0.006
23	20.805	1373	224	0.007
24	21.119	1159	203	0.006
25	22.214	1892	222	0.010

Peak#	Ret. Time	Area	Height	Area %
26	23.834	3365	488	0.018
27	24.380	3513	280	0.018
Total		19105343	1167461	100.000