

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E0974819K
 Time Processed :8:38:14 AM
 Month-Day-Year Processed :11/20/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

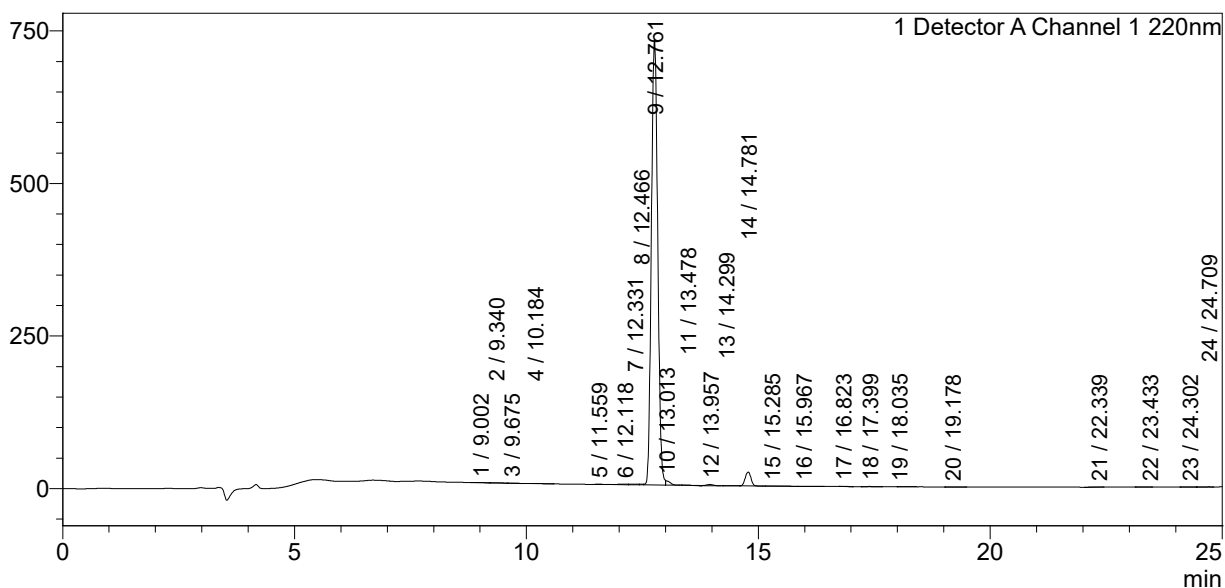

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.002	3392	277	0.047
2	9.340	3894	332	0.054
3	9.675	2259	191	0.031
4	10.184	4026	231	0.055
5	11.559	4717	641	0.065
6	12.118	12471	823	0.172
7	12.331	13742	1036	0.189
8	12.466	6376	1071	0.088
9	12.761	6931178	730873	95.417
10	13.013	45628	7240	0.628
11	13.478	3193	339	0.044
12	13.957	18572	1855	0.256
13	14.299	1516	74	0.021
14	14.781	194545	22613	2.678
15	15.285	3477	281	0.048

Peak#	Ret. Time	Area	Height	Area%
16	15.967	1775	97	0.024
17	16.823	1181	113	0.016
18	17.399	2855	255	0.039
19	18.035	2063	148	0.028
20	19.178	2316	141	0.032
21	22.339	1349	94	0.019
22	23.433	1168	97	0.016
23	24.302	1380	120	0.019
24	24.709	1034	79	0.014
Total		7264109	769021	100.000