

Sample Name : Chemerin-9(149-157)
 Cat. No. : RP20248
 Lot. No. : PE0321902
 Time Processed : 23:03:57
 Month-Day-Year Processed : 02/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

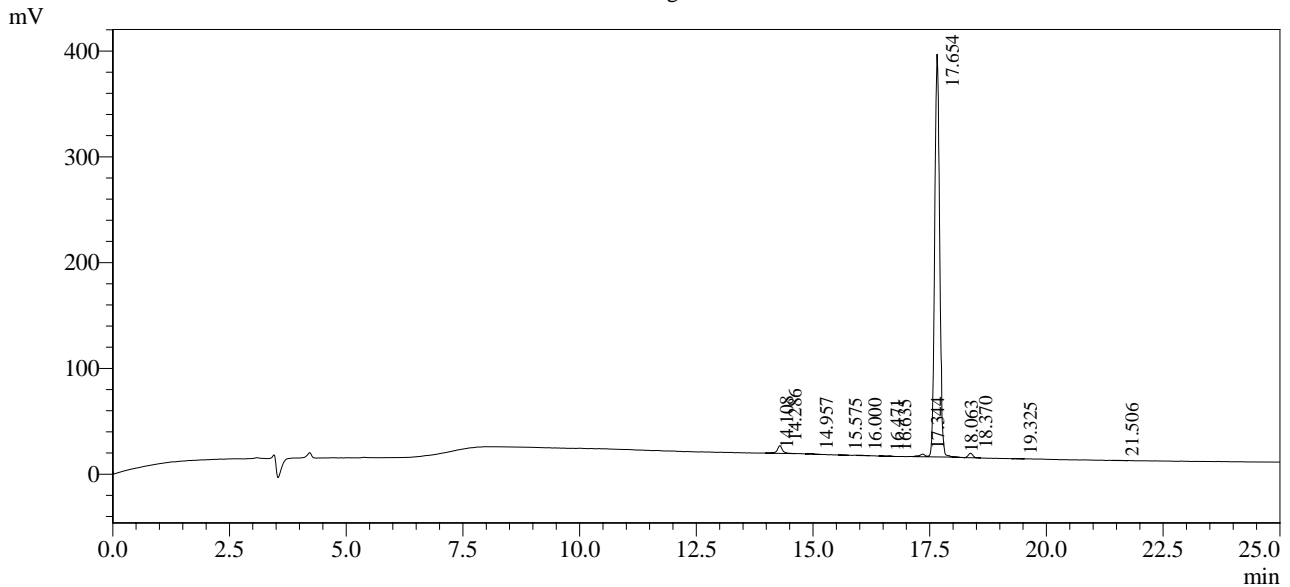

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.108	1848	368	0.063
2	14.286	53349	7224	1.815
3	14.957	3617	452	0.123
4	15.575	1098	184	0.037
5	16.000	3331	343	0.113
6	16.471	1738	257	0.059
7	16.635	3158	495	0.107
8	17.344	22430	2534	0.763
9	17.654	2813985	380620	95.733
10	18.063	1019	173	0.035
11	18.370	29466	4321	1.002
12	19.325	1534	174	0.052
13	21.506	2849	242	0.097
Total		2939421	397387	100.000