

Sample Name :HA Peptide
 Cat No. :RP11735
 Lot No. :E5964120C
 Time Processed :8:29:46
 Month-Day-Year Processed :03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

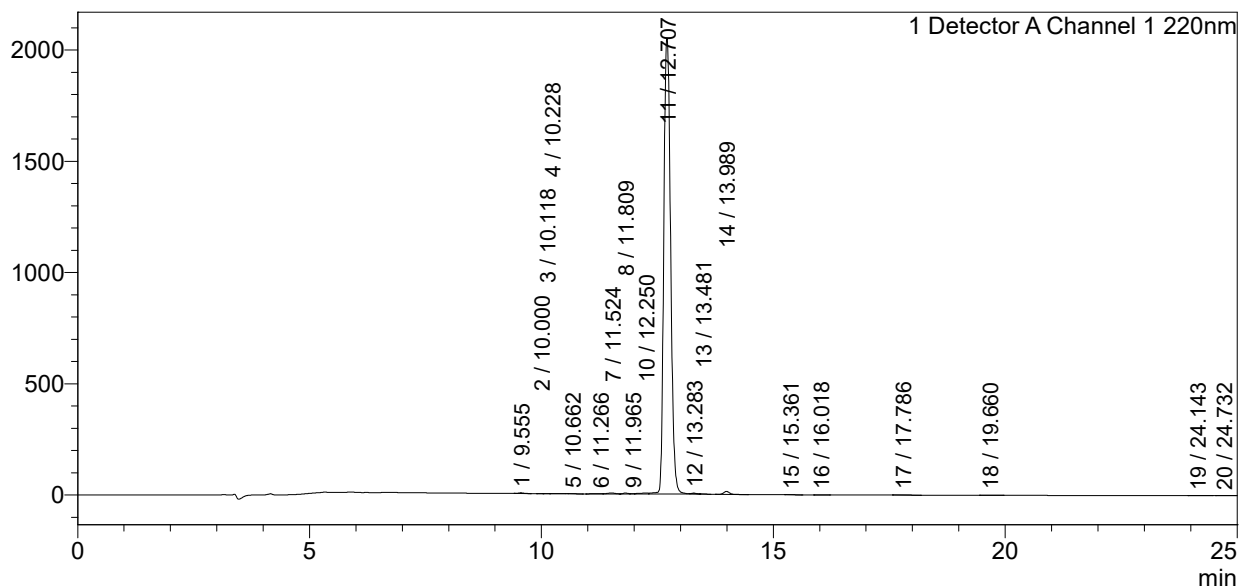

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.555	25262	3051	0.119
2	10.000	1296	246	0.006
3	10.118	4071	553	0.019
4	10.228	6205	751	0.029
5	10.662	1125	101	0.005
6	11.266	14069	1099	0.066
7	11.524	45824	3972	0.217
8	11.809	27660	4041	0.131
9	11.965	10642	1706	0.050
10	12.250	54251	3812	0.256
11	12.707	20792222	2049332	98.256
12	13.283	20055	3271	0.095
13	13.481	4872	815	0.023
14	13.989	127835	13887	0.604
15	15.361	2564	284	0.012

Peak#	Ret. Time	Area	Height	Area%
16	16.018	3654	439	0.017
17	17.786	9071	629	0.043
18	19.660	3045	190	0.014
19	24.143	4251	231	0.020
20	24.732	3363	216	0.016
Total		21161339	2088627	100.000