

Sample Name : β -Amyloid (1-40)
 Cat No :RP10004
 Lot No :E8209521C
 Time Processed :15:09:50
 Month-Day-Year Processed :04/23/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

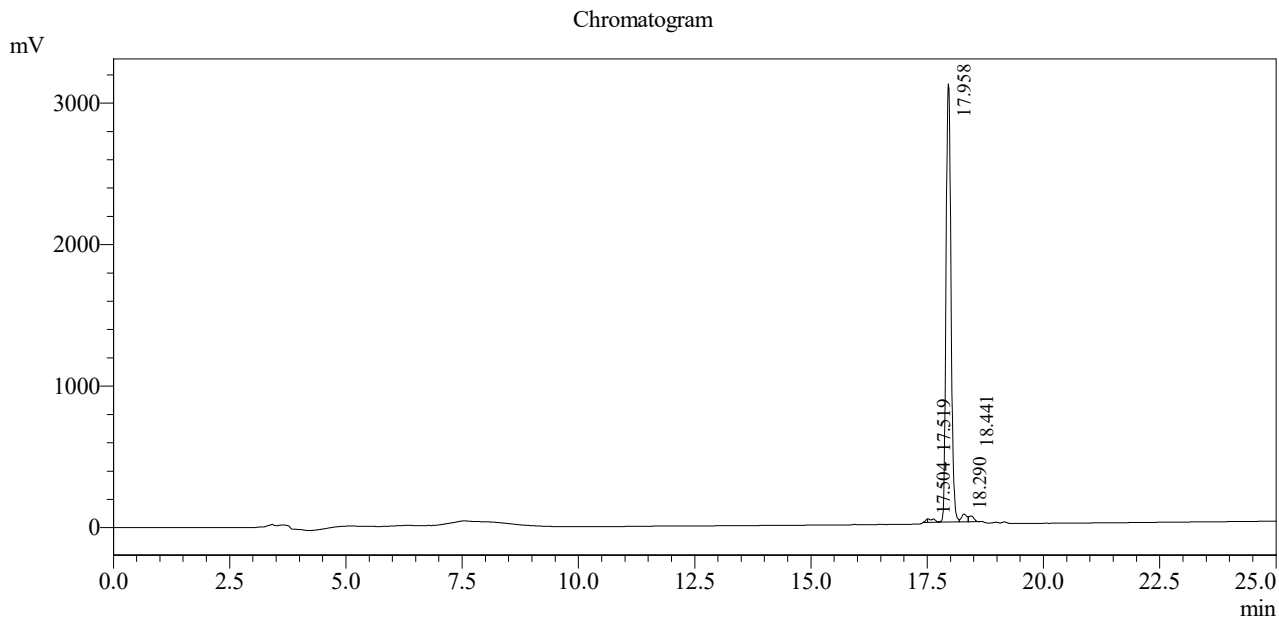

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.504	79889	23243	0.333
2	17.519	224653	24872	0.937
3	17.958	22938902	3095739	95.654
4	18.290	450210	54946	1.877
5	18.441	287589	40151	1.199
Total		23981244	3238951	100.000