

Sample Name : C-Type Natriuretic Peptide (CNP) (1-22), human
 Cat No.: RP11110
 Lot No.: E2086720E
 Time Processed : 10:00:34
 Month-Day-Year Processed : 05/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
30.00	Pumps	Pump A B.Conc	95
35.00	Pumps	Pump A B.Conc	95
35.10	Pumps	Pump A B.Conc	15
40.20	Pumps	Pump A B.Conc	15
41.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

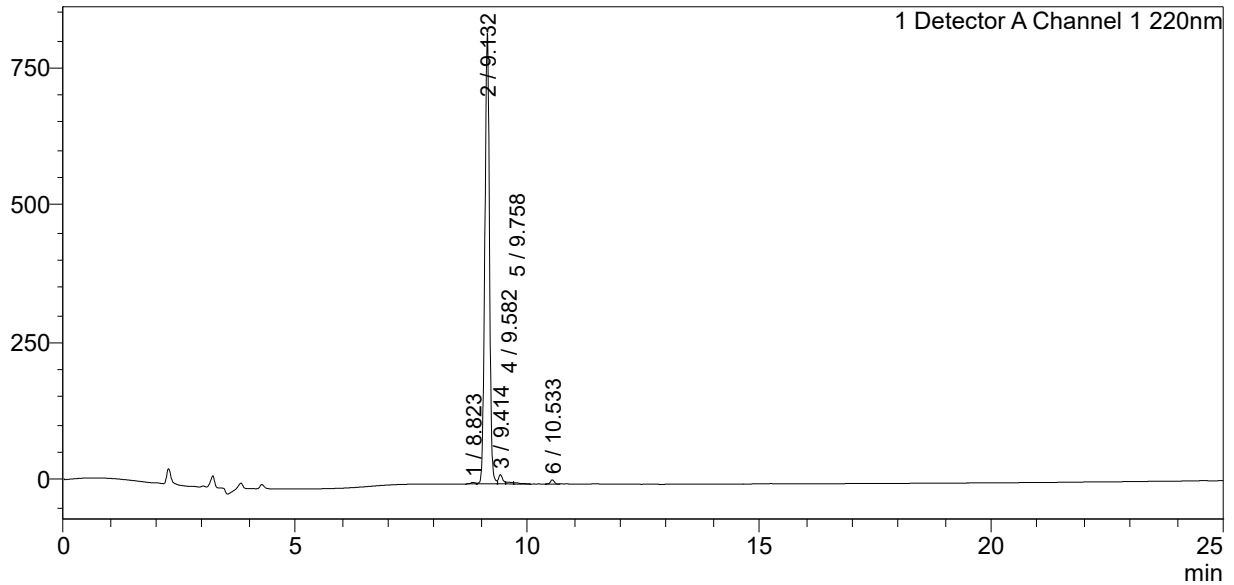

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.823	19874	2776	0.337
2	9.132	5667247	821267	96.145
3	9.414	118681	17147	2.013
4	9.582	25261	3112	0.429
5	9.758	20362	2214	0.345
6	10.533	43057	7599	0.730
Total		5894482	854115	100.000