

Sample Name :HA Peptide  
 Cat No. :RP11735  
 Lot No. :E4268720L  
 Time Processed :23:35:45  
 Month-Day-Year Processed :12/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

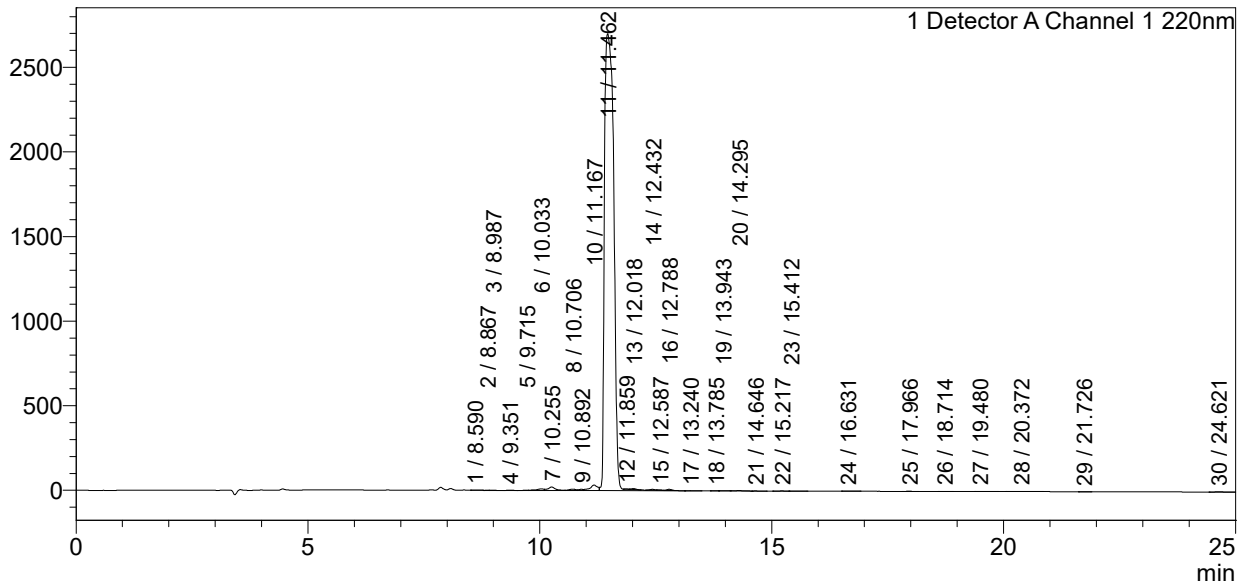

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.590	6480	794	0.017
2	8.867	1545	322	0.004
3	8.987	6095	951	0.016
4	9.351	16033	2281	0.042
5	9.715	12647	1660	0.033
6	10.033	111233	8830	0.289
7	10.255	235250	20586	0.611
8	10.706	85668	8549	0.222
9	10.892	48998	7141	0.127
10	11.167	375330	32784	0.974
11	11.462	37366839	2701301	96.974
12	11.859	9720	1990	0.025
13	12.018	42233	5960	0.110
14	12.432	40828	5231	0.106

Peak#	Ret. Time	Area	Height	Area%
15	12.587	20225	3136	0.052
16	12.788	56245	6917	0.146
17	13.240	4774	362	0.012
18	13.785	2437	314	0.006
19	13.943	5545	716	0.014
20	14.295	25655	2798	0.067
21	14.646	1983	284	0.005
22	15.217	6252	894	0.016
23	15.412	1876	43	0.005
24	16.631	3206	362	0.008
25	17.966	3385	344	0.009
26	18.714	1800	186	0.005
27	19.480	2486	119	0.006
28	20.372	23604	958	0.061
29	21.726	1641	232	0.004
30	24.621	12641	1298	0.033
Total		38532653	2817343	100.000