

Sample Name :OVA Peptide (323-339)  
 Cat No. :RP10610  
 Lot No. :E0163121D  
 Time Processed :11:50:04 PM  
 Month-Day-Year Processed :04/26/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

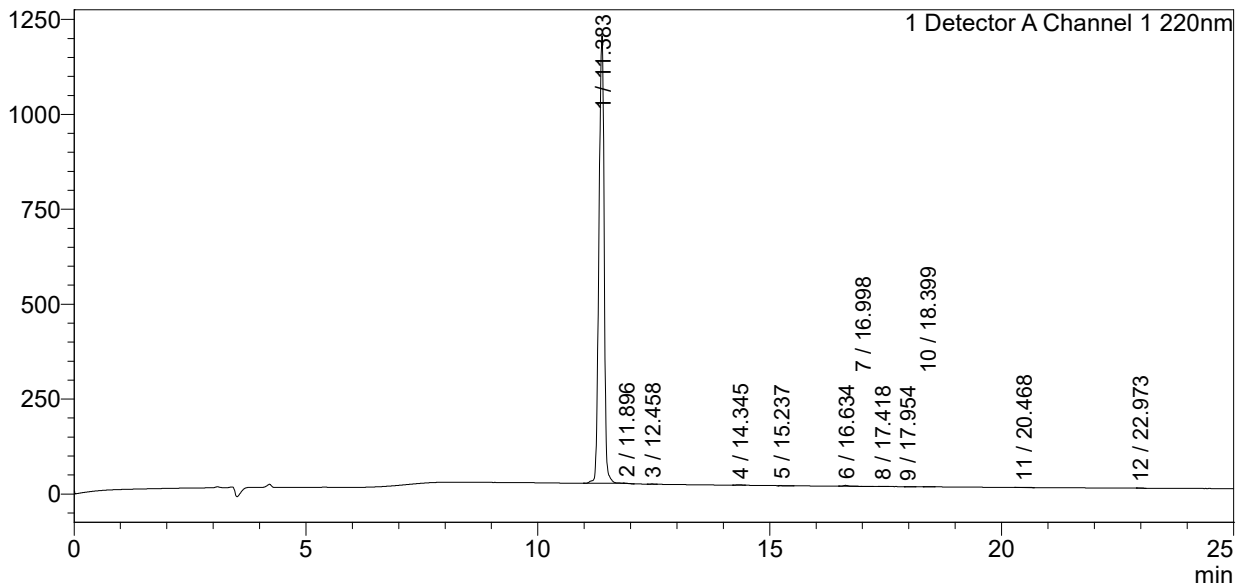

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.383	9155421	1179645	99.492
2	11.896	2846	489	0.031
3	12.458	3609	704	0.039
4	14.345	8736	1322	0.095
5	15.237	1490	163	0.016
6	16.634	18636	2375	0.203
7	16.998	1044	70	0.011
8	17.418	1661	328	0.018
9	17.954	1072	156	0.012
10	18.399	2841	459	0.031
11	20.468	3813	286	0.041
12	22.973	1042	192	0.011
Total		9202210	1186189	100.000