

Sample Name :LL37 (Human)
 Cat. No. : RP13323
 Lot. No. : PE0221903
 Time Processed : 11:10:16
 Month-Day-Year Processed : 03/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
48.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

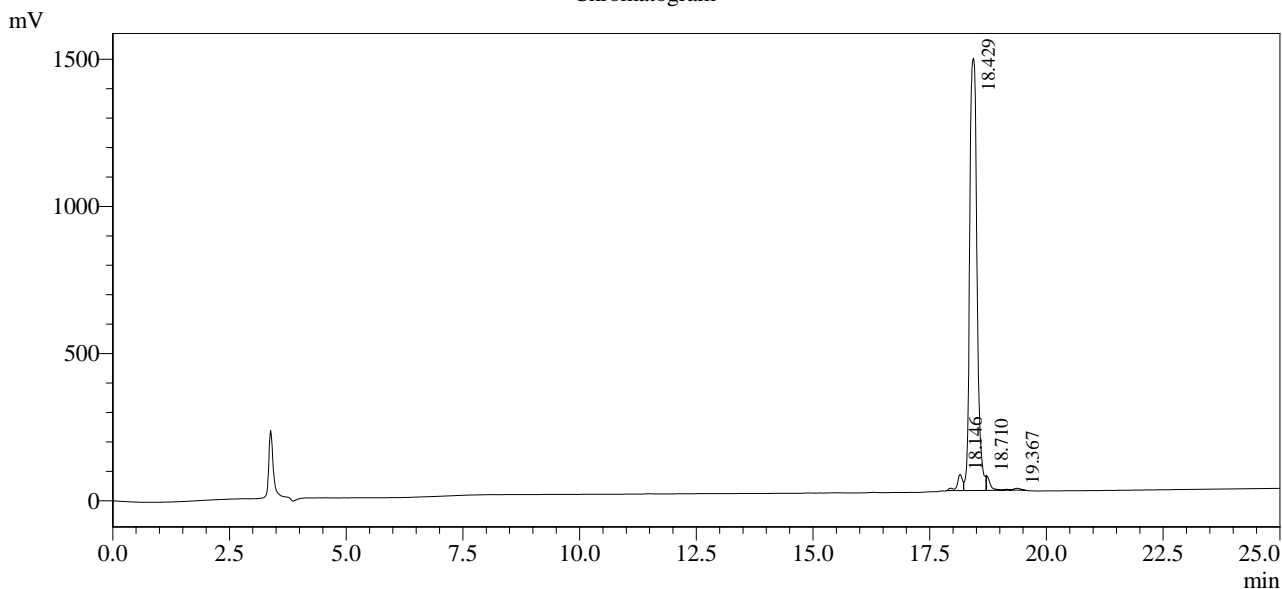

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	18.146	437601	54617	2.617
2	18.429	15925677	1468563	95.234
3	18.710	278152	49473	1.663
4	19.367	81277	6418	0.486
Total		16722707	1579070	100.000