

Sample Name :Melittin,honey bee
 Cat No. :RP20415
 Lot No. :E6142420J
 Time Processed :21:06:21
 Month-Day-Year Processed :10/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

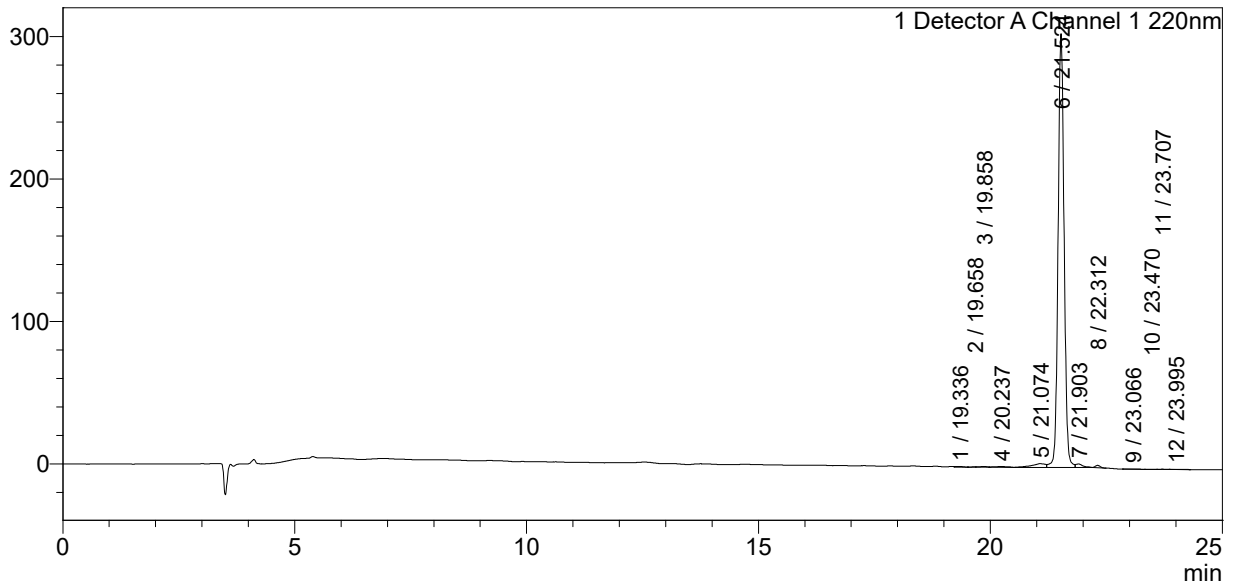

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	19.336	4290	368	0.150
2	19.658	1539	229	0.054
3	19.858	6085	580	0.213
4	20.237	10998	668	0.384
5	21.074	54387	2586	1.900
6	21.524	2740104	304383	95.714
7	21.903	25177	2390	0.879
8	22.312	11240	1626	0.393
9	23.066	3988	241	0.139
10	23.470	1199	137	0.042
11	23.707	1474	189	0.051
12	23.995	2309	180	0.081
Total		2862791	313576	100.000