

Sample Name: Glucagon (1-29), Human, Hydrochloride Salt
 Cat. No. : RP10772-0.5
 Lot No. : PE4011709

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

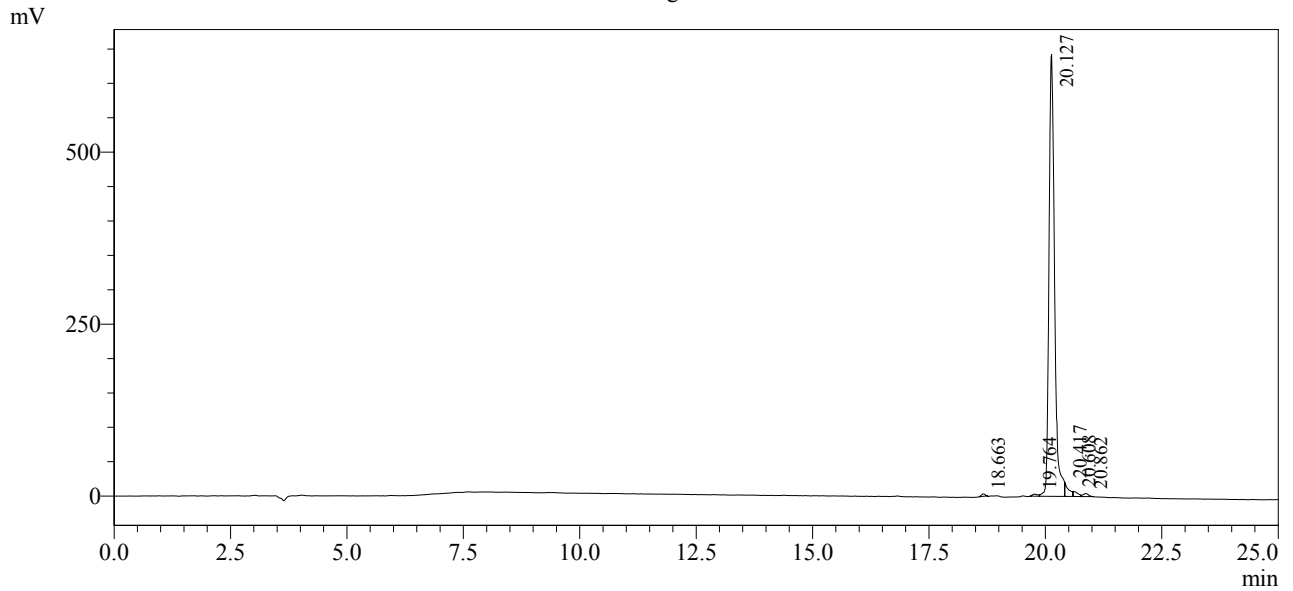

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	18.663	20741	3583	0.372
2	19.764	25081	2961	0.450
3	20.127	5335564	642371	95.680
4	20.417	109632	20365	1.966
5	20.608	49148	6794	0.881
6	20.862	36303	4425	0.651
Total		5576468	680500	100.000