

Sample Name : Substance P
 Cat No. : RP10178
 Lot No. : PE7351705

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	5
40.00	Pumps	Pump B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

<Chromatogram>

mV

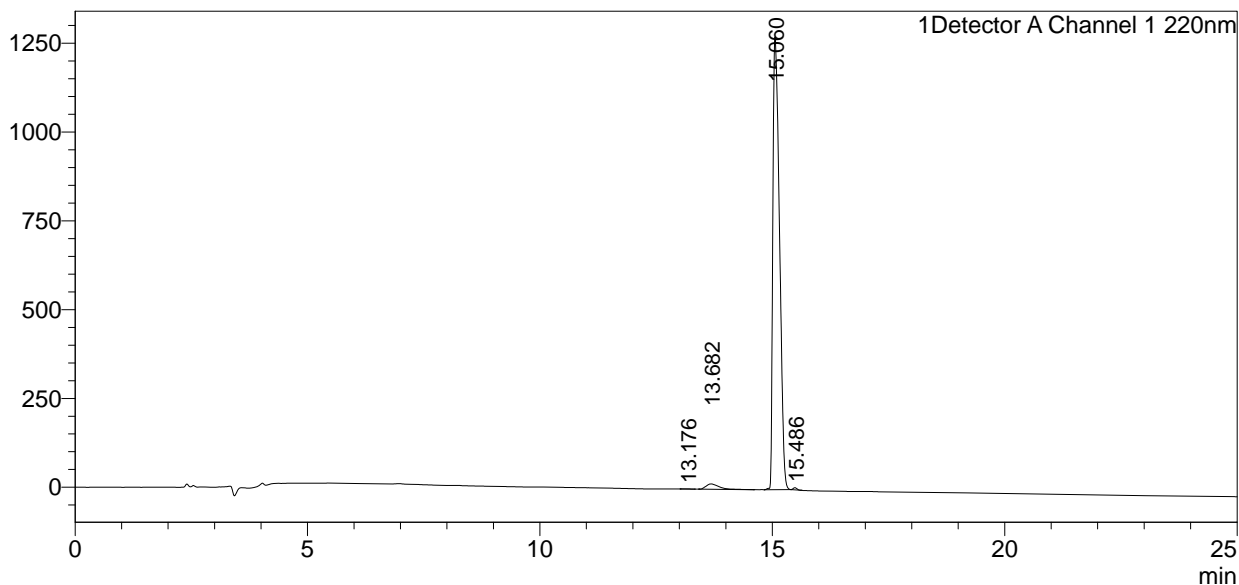

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.176	3449	464	0.027
2	13.682	295305	15140	2.275
3	15.060	12646562	1275003	97.437
4	15.486	33906	6173	0.261
Total		12979222	1296780	100.000