

Sample Name : β -Amyloid (1-42), human
 Cat. No. : RP20527
 Lot. No. : PE1901810
 Time Processed : 8:30:52
 Month-Day-Year Processed : 10/11/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	10	
25.00	Pumps	Pump B Conc.	100	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	10	
40.00	Pumps	Pump B Conc.	10	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : SS-CM-0310

Chromatogram

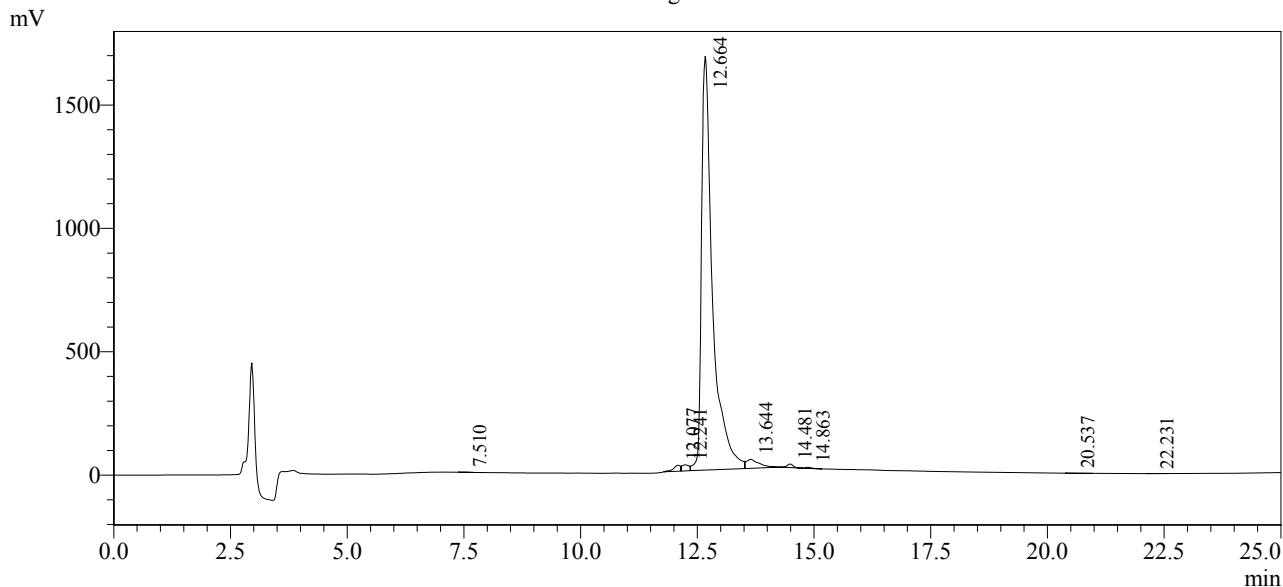

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.510	11964	1049	0.041
2	12.077	247996	24092	0.851
3	12.241	263192	24519	0.903
4	12.664	27723204	1677417	95.159
5	13.644	707168	36297	2.427
6	14.481	131538	14603	0.452
7	14.863	38650	4350	0.133
8	20.537	7526	497	0.026
9	22.231	2290	153	0.008
Total		29133528	1782976	100.000