

Sample Name:MDYKDHDGDYKDHDIDYKDDDDK peptide
 Cat No. :RP21087
 Lot No. :E5493321H
 Time Processed :1:35:50 PM
 Month-Day-Year Processed :08/18/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

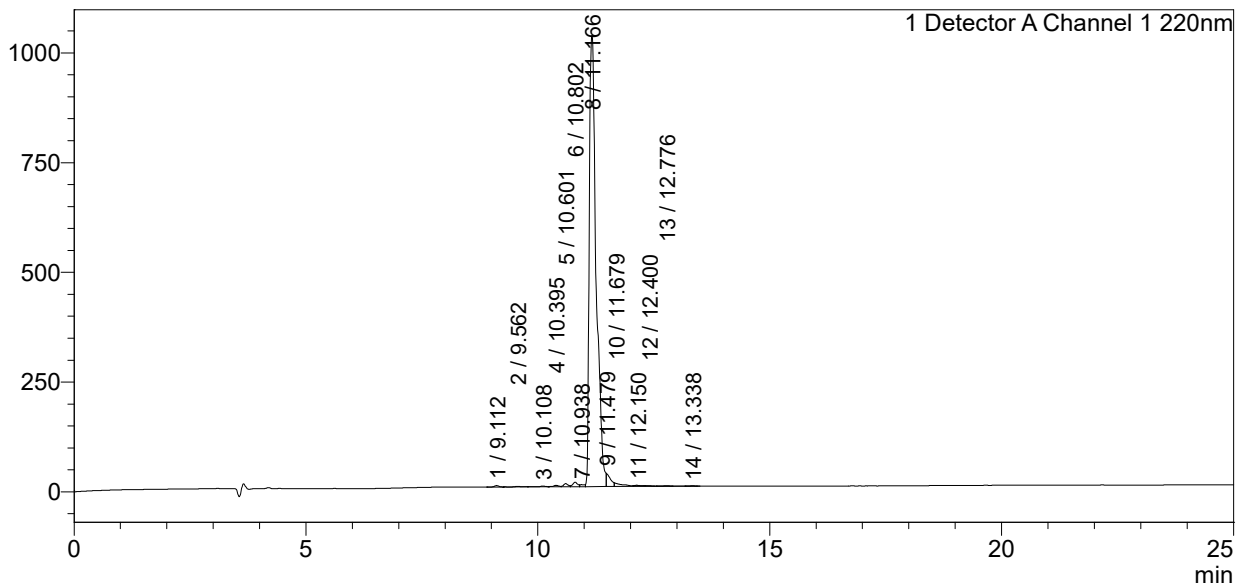

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.112	19049	2990	0.171
2	9.562	9418	1113	0.084
3	10.108	13909	1790	0.125
4	10.395	24922	3245	0.223
5	10.601	46909	6738	0.420
6	10.802	73273	9835	0.656
7	10.938	31982	4472	0.286
8	11.166	10613817	1023997	95.032
9	11.479	186342	31020	1.668
10	11.679	131779	7644	1.180
11	12.150	7232	1154	0.065
12	12.400	1479	341	0.013
13	12.776	5477	592	0.049
14	13.338	3088	428	0.028

Peak#	Ret. Time	Area	Height	Area%
Total		11168676	1095360	100.000