


Mass Spectrum

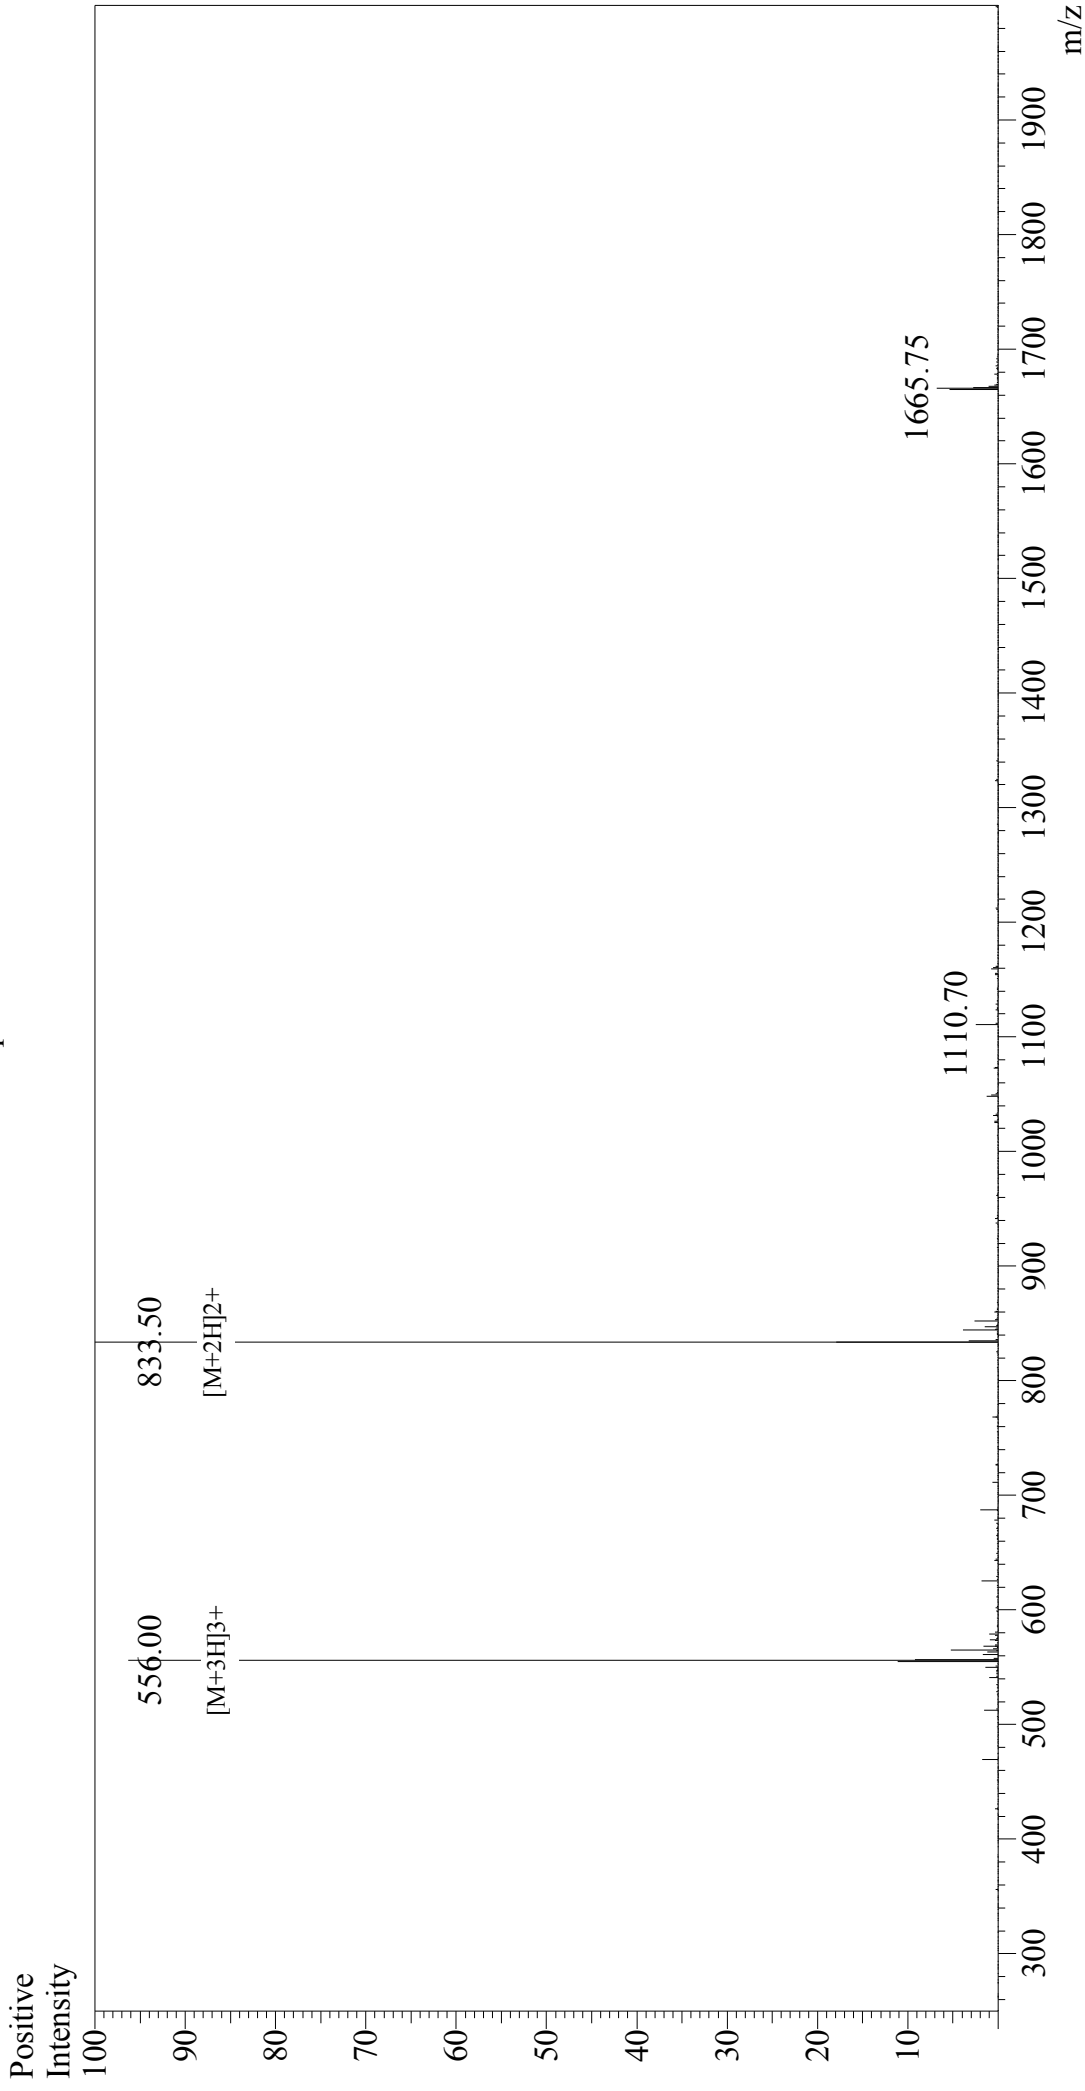

Sample Information

Acquired by : Gary
Month-Day Processed : 10/12/17
Time Processed : 19:16:20
Injection Volume : 0.2
Sample Name : α -Melanocyte-Stimulating Hormone (MSH), amide
Cat. No. : RP10644
Lot. No. : PE3291710
Theoretical MW : 1664.90
Observed MW : 1665.00

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH