

Sample Name :Neuropeptide Y, human
 Cat No. :RP10492
 Lot No. :E8748820K
 Time Processed :8:57:07
 Month-Day-Year Processed :12/01/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

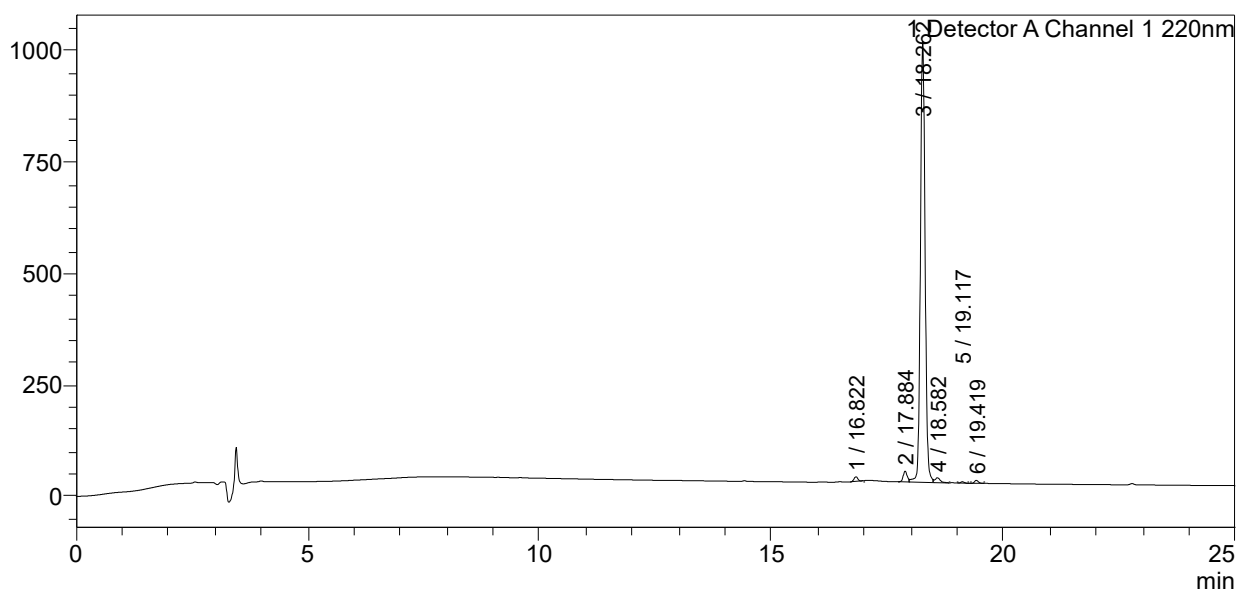

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.822	56491	10116	0.772
2	17.884	147940	23802	2.023
3	18.262	6975801	990866	95.382
4	18.582	79101	10959	1.082
5	19.117	16600	3138	0.227
6	19.419	37630	6554	0.515
Total		7313563	1045435	100.000