

Sample Name: Glucagon (1-29), Human  
 Cat No. : RP10772  
 Lot No. : E8522820F  
 Time Processed: 1:05:06 PM  
 Month-Day-Year Processed :06/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment: ZJ19010325

<Chromatogram>

mV

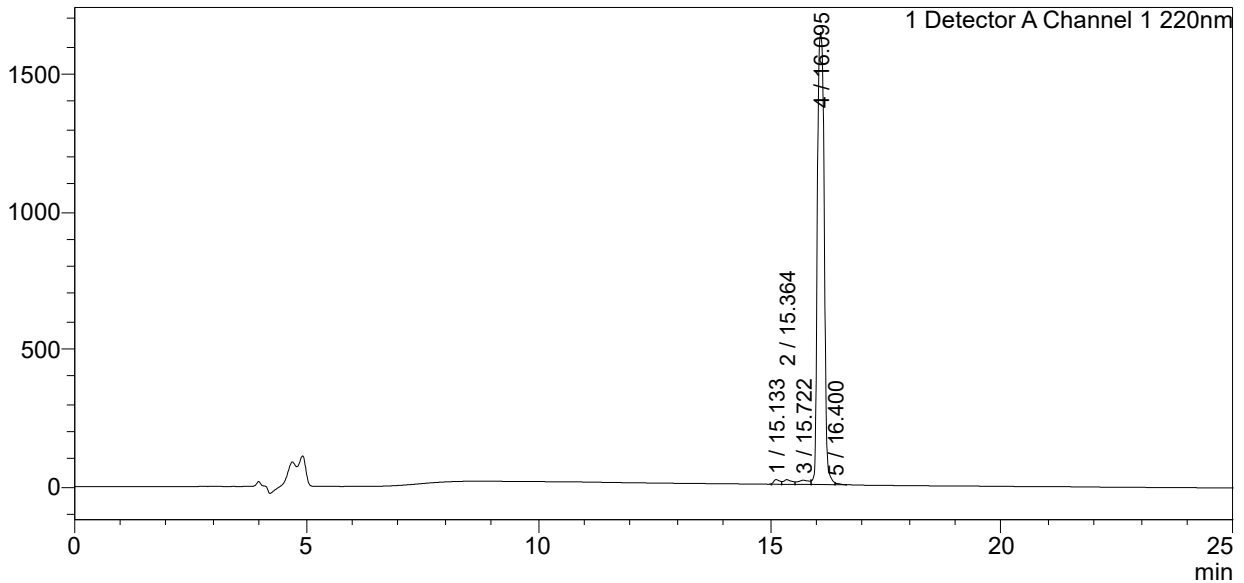

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.133	164138	16857	0.950
2	15.364	212595	16864	1.230
3	15.722	257666	15164	1.491
4	16.095	16615127	1645231	96.118
5	16.400	36640	7226	0.212
Total		17286167	1701342	100.000