

Sample Name :LAH4
 Cat. No. :RP20096
 Lot. No. :E8575719H
 Time Processed :5:36:16 AM
 Month-Day-Year Processed :08/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

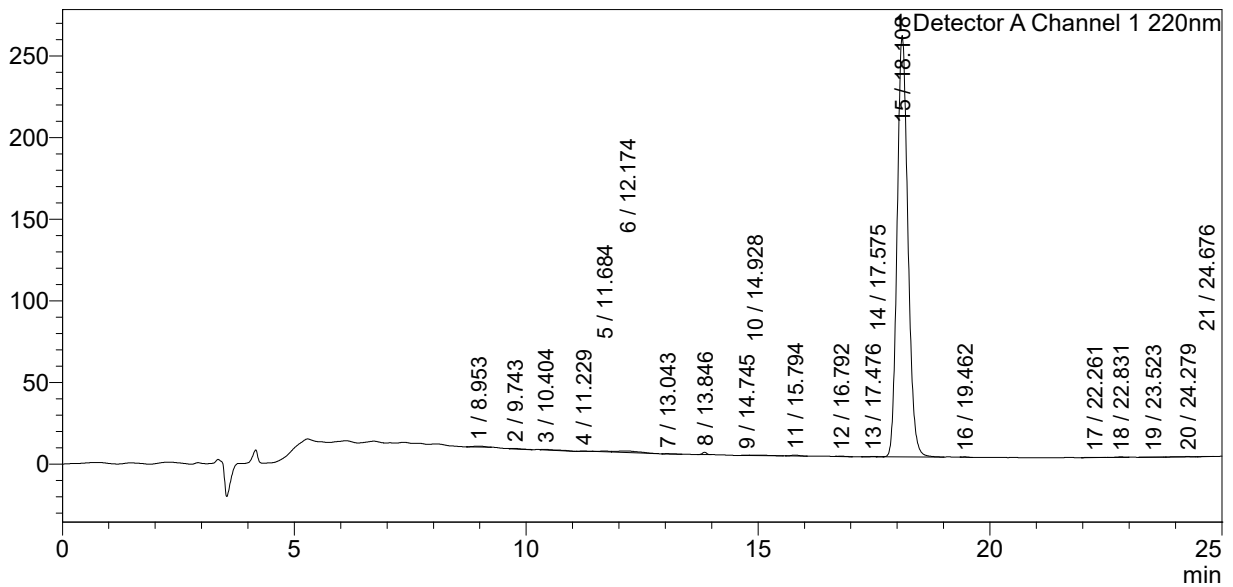

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.953	9653	541	0.225
2	9.743	3143	238	0.073
3	10.404	11858	356	0.277
4	11.229	2025	191	0.047
5	11.684	7829	447	0.183
6	12.174	34644	986	0.808
7	13.043	1524	123	0.036
8	13.846	9257	1452	0.216
9	14.745	1683	179	0.039
10	14.928	7776	302	0.181
11	15.794	6009	519	0.140
12	16.792	1763	160	0.041
13	17.476	2230	182	0.052
14	17.575	1215	163	0.028
15	18.108	4170469	258336	97.286

Peak#	Ret. Time	Area	Height	Area%
16	19.462	1482	229	0.035
17	22.261	2234	118	0.052
18	22.831	4197	315	0.098
19	23.523	2370	133	0.055
20	24.279	4038	173	0.094
21	24.676	1403	112	0.033
Total		4286803	265255	100.000