

Sample Name : Exendin-4
 Cat No. : RP10874
 Lot No. : E8894121F
 Time Processed : 18:10:42
 Month-Day-Year Processed : 07/03/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

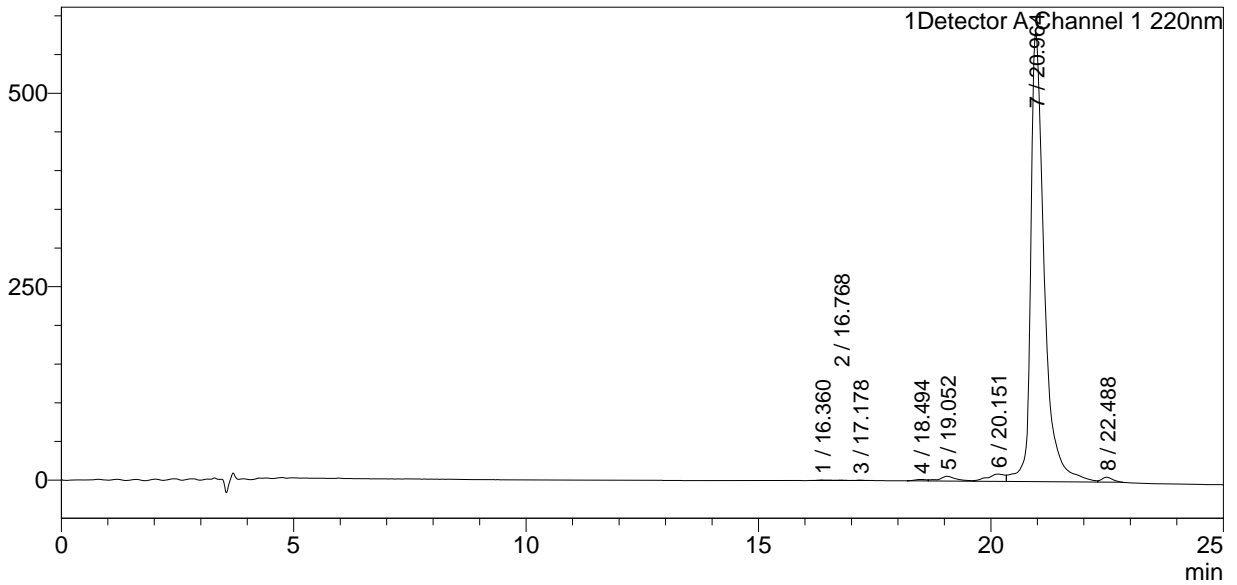

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.360	10963	575	0.089
2	16.768	5339	464	0.043
3	17.178	4514	555	0.037
4	18.494	31792	1900	0.258
5	19.052	158261	6174	1.282
6	20.151	246949	9478	2.000
7	20.964	11783598	579930	95.447
8	22.488	104330	6285	0.845
Total		12345747	605361	100.000