

Sample Name :Cortistatin 14, human, rat  
 Caty No.: RP10972 Lot No.: PE3361709

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

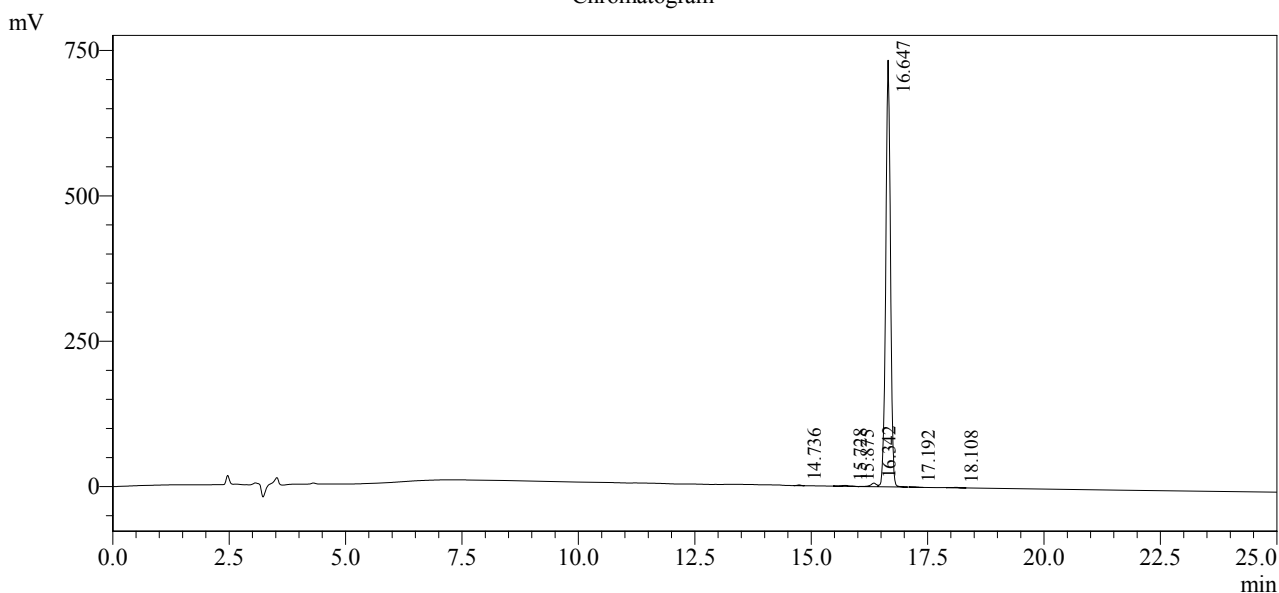

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.736	7230	1318	0.137
2	15.728	15078	1585	0.285
3	15.875	3912	691	0.074
4	16.342	54826	6286	1.038
5	16.647	5192137	733565	98.267
6	17.192	2094	244	0.040
7	18.108	8435	978	0.160
Total		5283712	744668	100.000